



## Installation and operating instructions portable dew point meters DP 500 / DP 510



### I. Foreword

Dear customer,

thank you very much for deciding in favour of the DP 500 / DP 510. Please read this installation and operation manual carefully before mounting and initiating the device and follow our advice. A riskless operation and a correct functioning of the DP 500 / DP 510 are only guaranteed in case of careful observation of the described instructions and notes



#### **Sales Office South / Geschäftsstelle Süd**

Zindelsteiner Str. 15

D-78052 VS-Tannheim

Tel.: +49 (0) 7705 978 99 0

Fax: +49 (0) 7705 978 99 20

Mail: [info@cs-instruments.com](mailto:info@cs-instruments.com)

Web: <http://www.cs-instruments.com>

#### **Sales Office North / Geschäftsstelle Nord**

Am Oxer 28c

D-24955 Harrislee

Tel.: +49 (0) 461 700 20 25

Fax: +49 (0) 461 700 20 26

Mail: [info@cs-instruments.com](mailto:info@cs-instruments.com)

Web: <http://www.cs-instruments.com>

## Table of Contents

---

### II. Table of Contents

|  |           |
|--|-----------|
| <b>II. TABLE OF CONTENTS</b>   | <b>3</b>  |
| <b>1 SAFETY INSTRUCTIONS</b>   | <b>6</b>  |
| <b>2 APPLICATION AREA</b>  | <b>7</b>  |
| <b>3 TECHNICAL DATA DP 500 / DP 510</b>  | <b>8</b>  |
| <b>4 INSTALLATION AND MEASUREMENTS</b>   | <b>9</b>  |
| 4.1 Measurement with measuring chamber, connection via plug nipple               | 9         |
| 4.2 Measurement without measuring chamber, connection via external thread G1/2"  | 9         |
| 4.3 Dew point measuring at synthetic granules -dries                             | 10        |
| <b>5 MAINTENANCE</b>   | <b>10</b> |
| <b>6 CALIBRATION / ADJUSTMENT</b>  | <b>10</b> |
| <b>7 INPUTSIGNALS EXT. SENSOR DP 510</b>   | <b>11</b> |
| <b>8 CABLE CROSS SECTION</b>   | <b>11</b> |
| 8.1 Sensor circuit points/Output signal:   | 11        |
| <b>9 CONNECTION DIAGRAMS OF THE DIFFERENT SENSOR TYPs (DP 510 ONLY)</b>          | <b>12</b> |
| 9.1 Connector pin assignment for all sensors DP 510                              | 12        |
| 9.2 Connection CS dew point sensors series FA 415/FA 300                         | 13        |
| 9.3 Connection for CS dew point- and consumption sensors, series FA/VA 400       | 13        |
| 9.4 Connection for CS dew point- and consumption sensors, series FA/VA 5xx       | 13        |
| 9.5 Connection pulse sensors   | 14        |
| 9.6 Analogue two-, three-, and four-wire current signal                          | 15        |
| 9.7 Three- and four-wire power supply 0 - 1/10/30 VDC                            | 16        |
| 9.8 Two-, three-, and four-wire connector pin assignments for PT100/PT1000/KTY81 | 17        |
| 9.9 Connection with RS485  | 17        |

# Table of Contents

---

|                |   |           |
|----------------|---|-----------|
| <b>10</b>      | <b>OPERATION DP 500 / DP 510</b>                                | <b>18</b> |
| <b>10.1</b>    | <b>Keypad</b>   | <b>18</b> |
| 10.1.1         | On- and Off button  | 18        |
| 10.1.2         | Brightness buttons  | 18        |
| 10.1.3         | Screenshot-Button   | 18        |
| 10.1.3.1       | Storing Screenshot  | 18        |
| 10.1.3.2       | Export Screenshots  | 19        |
| <b>10.2</b>    | <b>Touchpanel</b>   | <b>21</b> |
| <b>10.3</b>    | <b>Main menu (Home)</b>   | <b>22</b> |
| 10.3.1         | Initialization  | 22        |
| 10.3.2         | Main menu   | 23        |
| 10.3.2.1       | Settings  | 24        |
| 10.3.2.1.1     | Password-Settings   | 24        |
| 10.3.2.1.2     | Sensor-settings   | 25        |
| 10.3.2.1.2.1   | Settings internal Dew point-Sensor                              | 26        |
| 10.3.2.1.2.1.1 | Definition of the System pressure (relative pressure value)     | 26        |
| 10.3.2.1.2.1.2 | Definition of Reference pressure (absolute pressure value)      | 27        |
| 10.3.2.1.2.2   | Choice of the sensor type (For example type CS-Digital sensor)  | 28        |
| 10.3.2.1.2.3   | Label and setting the description fields                        | 28        |
| 10.3.2.1.2.4   | Name the measurement data and define the decimal places         | 29        |
| 10.3.2.1.2.5   | Recording measurement data                                      | 29        |
| 10.3.2.1.2.6   | Alarm-Settings ( Alarm Popup)                                   | 30        |
| 10.3.2.1.2.7   | More Settings (scale analogue output)                           | 31        |
| 10.3.2.2       | Dew Point Sensor FA 400 / FA 410 of type CS-Digital (SDI Bus)   | 32        |
| 10.3.2.3       | Flow sensor VA 400 / VA 420 of type CS-Digital (SDI Bus)        | 33        |
| 10.3.2.4       | Dew Point Sensor FA 500 / FA 510 of type FA 5xx (RS 485 Modbus) | 36        |
| 10.3.2.4.1     | Settings Dew point sensor FA 500 FA 510                         | 37        |
| 10.3.2.4.1.1   | Unit selection for temperature and humidity                     | 37        |
| 10.3.2.4.1.2   | Definition of the System pressure (relative pressure value)     | 37        |
| 10.3.2.4.1.3   | Definition of Reference pressure (absolute pressure value)      | 38        |
| 10.3.2.4.2     | Calibration   | 38        |
| 10.3.2.4.3     | More Settings Analogue output 4-20mA                            | 39        |
| 10.3.2.5       | Flow sensor of type VA 5xx (RS 485 Modbus)                      | 40        |
| 10.3.2.5.1     | Settings for Flow sensor VA 5xx                                 | 41        |
| 10.3.2.5.1.1   | Diameter settings   | 41        |
| 10.3.2.5.1.2   | Gas Constant settings   | 42        |
| 10.3.2.5.1.3   | Definition of the reference conditions                          | 43        |
| 10.3.2.5.1.4   | Definition Unit of flow and velocity                            | 43        |
| 10.3.2.5.1.5   | Definition consumption counter value and consumption unit       | 43        |
| 10.3.2.5.2     | Settings analogue output 4-20mA of VA 5xx                       | 45        |
| 10.3.2.5.3     | Settings Pulse / Alarm output of VA 5xx                         | 46        |
| 10.3.2.5.4     | Settings ZeroPoint or Low Flow Cut off for VA 5xx               | 47        |
| 10.3.2.5.4.1   | Configuration of Analog-Sensors                                 | 48        |
| 10.3.2.5.4.2   | Type 0 - 1/10/30 Volt and 0/4 – 20 mA                           | 48        |
| 10.3.2.5.4.3   | Type PT100x and KTY81   | 50        |
| 10.3.2.5.4.4   | Type Pulse (Pulse ration)                                       | 51        |
| 10.3.2.5.4.5   | Type „No Sensor“  | 53        |
| 10.3.2.5.4.6   | Type Modbus   | 54        |
| 10.3.2.5.4.7   | Selection and activation of Sensor-Type Modbus                  | 54        |
| 10.3.2.5.4.7.1 | Modbus Settings   | 54        |
| 10.3.2.5.5     | Data logger Settings  | 58        |

## Table of Contents

---

|                |  |           |
|----------------|--|-----------|
| 10.3.2.5.6     | Device Settings  | 62        |
| 10.3.2.5.6.1   | Language   | 62        |
| 10.3.2.5.6.2   | Date & Time  | 63        |
| 10.3.2.5.6.3   | SD-Card  | 64        |
| 10.3.2.5.6.4   | System update  | 65        |
| 10.3.2.5.6.4.1 | Save System Settings   | 65        |
| 10.3.2.5.6.4.2 | Check for new Software updates (USB)                             | 66        |
| 10.3.2.5.6.5   | Factory Reset  | 67        |
| 10.3.2.5.6.6   | Calibrate touch-screen   | 68        |
| 10.3.2.5.7     | Cleaning   | 68        |
| 10.3.2.5.8     | System-Status  | 68        |
| 10.3.2.5.9     | About DP 500 / DP 510  | 69        |
| 10.3.2.6       | Chart  | 70        |
| 10.3.2.7       | Chart / Real time values   | 74        |
| 10.3.2.8       | Channels   | 76        |
| 10.3.2.8.1     | Min/Max Function   | 76        |
| 10.3.2.9       | Real time values   | 78        |
| 10.3.2.10      | Alarm overview   | 79        |
| <b>11</b>      | <b>VIRTUAL CHANNELS (OPTIONAL)</b>                               | <b>80</b> |
| 11.1           | Option „Virtual Channels“ activation                             | 80        |
| 11.2           | Virtual Channels Settings  | 81        |
| 11.2.1         | Selection of Sensor-type   | 81        |
| 11.2.2         | Configuration of each single virtual value                       | 82        |
| 11.2.3         | Activation of a single virtual value                             | 82        |
| 11.2.4         | Definition of Operands   | 82        |
| 11.2.5         | Definition of Operations   | 84        |
| 11.2.6         | Definition of Unit   | 84        |
| 11.2.7         | Value name, resolution of decimal places and recording of values | 86        |
| <b>12</b>      | <b>ANALOG TOTAL (OPTIONAL ONLY FOR DP 510)</b>                   | <b>87</b> |
| 12.1           | Option „Analog Total“ activation                                 | 87        |
| 12.2           | Selection of sensor type   | 88        |
| <b>13</b>      | <b>EXPORT /IMPORT</b>  | <b>89</b> |
| 13.1           | Export Logger data   | 89        |
| 13.2           | Export System Settings   | 91        |
| 13.3           | Import System Settings   | 92        |

### 1 Safety instructions



**Please check whether this manual corresponds with the device type.**

Please attend to all notes indicated in this instruction manual. It contains essential information which has to be followed during installation, operation and maintenance. Therefore, this instruction manual has to be read categorically by the technician as well as by the responsible user/qualified personnel before installation, initiation and maintenance.

This instruction manual has to be available at any time at the operation site of the DP 500 / DP 510. Regional and national regulations respectively, have to be observed in addition to this instruction manual if necessary.

In case of any obscurities or questions with regard to this manual or the instrument please contact CS Instruments GmbH.



**Warning!**

**Supply voltage!**

**Contact with supply voltage carrying non-insulated parts may cause an electric shock with injury and death.**

**Measures:**

- Note all applicable regulations for electrical installations (e.g. VDE 0100)!
- **Carry out maintenance only in strain less state!**
- All electric works are only allowed to be carried out by authorized qualified personnel.



**Warning!**

**Inadmissible operating parameters!**

**Undercutting and exceeding respectively of limit values may cause danger to persons and material and may lead to functional and operational disturbances.**

**Measures:**

- Make sure that the DP 500 / DP 510 is only operated within the admissible limit values indicated on the type label.
- Strict observance of the performance data of the DP 500 / DP 510 in connection with the application.
- Do not exceed the admissible storage and transportation temperature.

**Further safety instructions:**

- Attention should also be paid to the applicable national regulations and safety instructions during installation and operation.
- The DP 500 / DP 510 is not allowed to be used in explosive areas.

**Additional remarks:**

- Do not overheat the instrument!
- In case of mounting by screwing please use spanner flat (SW27)!
- DP 500 / DP 510 is not allowed to be disassembled!



**Attention!**

**Malfunctions at the DP 500 / DP 510!**

**Faulty installation and insufficient maintenance may lead to malfunctions of the DP 500 / DP 510 which may affect the measuring results and which may lead to misinterpretations.**

### 2 Application Area

The new instruments DP 500/DP510 are the ideal portable service instruments for dew point measurement for all types of driers down to -80°Ctd dew point

The 3.5" graphic display with touch screen makes the operation very easy.

The graphic indication of coloured measuring curves is unique.

Ideal for measurement of the current dew point and for graphic indication of the dew point curve/the switching behaviour of the drier over a longer period of time.

Up to 100 million measured values can be stored with date and measuring site name. The measured data can be transferred to the computer via USB stick or USB cable.

**DP 510** additionally disposes of one further freely assignable sensor input.

Apart from the internal dew point measurement, one further optional sensor can be connected like for example:

- Pressure sensors
- Flow sensors, VA 400/420
- Temperature sensors Pt 100, 4..20 mA
- Further dew point sensors
- Effective power meters
- Optional third-party sensors with the following signals:  
0...1/10 V, 0/4...20 mA, Pt100, Pt1000, pulse, Modbus

Application ranges:

- Compressed air: Examination of refrigeration, membrane, adsorption driers
- Technical gases: Residual moisture measurement in gases like N<sub>2</sub>, O<sub>2</sub> and so on
- Plastics industry: Examination of granulate driers
- Medical compressed air/breathing air

3 Technical data DP 500 / DP 510

|                                       |  |
|---------------------------------------|--|
| <b>CE</b>                             |  |
| Colour screen                         | 3.5"-Touchpanel TFT transmissive, graphics, curves, statistics   |
| Interfaces                            | USB  |
| Measuring ranges                      | -80...+50 °Ctd<br>-20...+70 °C<br>0...100 % rF   |
| Accuracy                              | ± 0,5 °Ctd (-10...+50 °Ctd)<br>typical: ± 2 °Ctd   |
| Humidity measures                     | g/m <sup>3</sup> , mg/m <sup>3</sup> , ppm V/V, g/kg, °Ctdatm, % rF  |
| Response Time T95                     | -50°Ctd ---- -10°Ctd < 10sec<br>-10°Ctd ---- -50°Ctd < 5 minutes   |
| Pressure range                        | Mounting without measuring chamber: -1...50 bar Standard<br>Mounting with measuring chamber: : 2...16 bar<br>High pressure version up to 350 bar                                 |
| Power supply for sensors (only DP510) | Output voltage: 24 VDC ± 10%<br>Output current: 120 mA continuous operation  |
| Current supply                        | Internal rechargeable Li-Ion batteries charging time approx. 4 h<br>DP 500 operation: approx. 12h,<br>DP 510 operation: > 4h depending on current consumption of external sensor |
| Power supply unit                     | 100 – 240 VAC/50 – 60 Hz, 12VDC – 1A<br>Safety class 2, only for application in dry rooms  |
| Dimensions                            | 125 x 96 x 245 mm  |
| Material                              | Plastic PC/ABS   |
| Weight                                | 550 g  |
| Operating temperature                 | -20...70°C measuring gas temperature<br>0... 50°C ambient temperature  |
| Storage temperature                   | -20 to +70°C   |
| Optional                              | Data Logger, Memory size 2 GB SD memory card standard, optionally up to 4 GB   |
| EMC                                   | DIN EN 61326   |



### 4 Installation and measurements

**We recommend the use of a measuring chamber!**

#### 4.1 Measurement with measuring chamber, connection via plug nipple



1. Preparation of the measuring point

Let compressed air flow off at the sampling point before measurement in order to remove condensate and particles. This avoids a soiling of DP 500 / DP 510 and the measuring chamber.

Stagnant air leads to long adjustment times.

If condensate occurs at the measuring point, please check the compressed-air conditioning before measurement.

2. Switch on DP 500 / DP 510 and wait until the initialization has been finished.

Please observe the chapter "Operation".

3. Connect the measuring chamber screwed onto DP 500 / DP 510 with the plug nipple coupling of the measuring point

4. Wait until the value in the display of DP 500 / DP 510 has stabilized. Depending on the position of the measuring point this may take up to 15 minutes.

5. Disconnect the measuring chamber from the plug nipple coupling of the measuring point after measurement. Switch off DP 500 / DP 510 if you do not want to carry out further measurements.

#### 4.2 Measurement without measuring chamber, connection via external thread G1/2"



1. Preparation of the measuring point

Make sure that the measuring point is depressurized.

Please check the sampling point before measurement.

If condensate occurs at the measuring point you should check the compressed-air conditioning before measurement.

2. Screw the DP 500 / DP 510 (without mounted measuring chamber) into the measuring point (with internal thread G1/2"). For mounting you should use the spanner flat (SW27)!

3. Switch on DP 500 / DP 510 and wait until the initialization has been finished.

Please observe the chapter "Operation".

4. Charge the measuring point slowly with pressure.


5. Wait until the value in the display of DP 500 / DP 510 has stabilized. Depending on the position of the measuring point this may take up to 15 minutes.

6. After measurement please drain the pressure slowly from the measuring point.

7. Remove DP 500 / DP 510 from the measuring point. For demounting the instrument, you should use the spanner flat (SW 27)!

8. If you do not want to carry out further measurements please switch off DP 500 / DP 510.

### 4.3 Dew point measuring at synthetic granules -dries

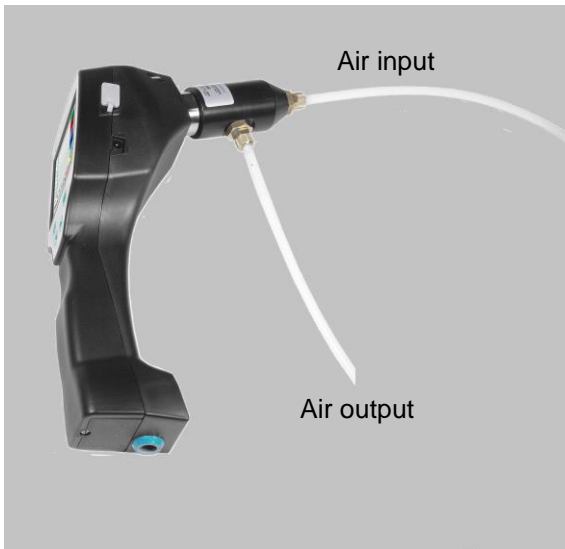

Synthetic granules-dries usually work with a slight positive pressure in the millibar range. Use in this application, with a slight excess pressure, the measuring chamber for synthetic granules dryer (Order No. 0699.3490).

Since the air temperature in the synthetic granules dryer is also very high, the air supply from the synthetic granules dryer to the measuring chamber via a correspondingly long Teflon tube (recommended length of 1-2 m), which serves as a cooling section. Note that the measured air temperature in the DP 500 if possible remains below 40 ° C, otherwise please use a longer Teflon tube as a cooling section.

The supply of air into the measuring chamber via port A (air input). On the air output, a Teflon tube is connected with a length of at least 80 cm. This prevents the back flow of humid ambient air back into the measuring chamber.

## 5 Maintenance

### Cleaning of the sensor

The sensor can be cleaned by careful swinging in distilled water or isopropanol.



**Remark:**

Do not touch the surface of the sensor pad.

Avoid mechanical impact to the sensor (e.g. by means of a sponge or a brush).

If the sensor is much polluted the only possibility will be an examination and maintenance by the manufacturer.

## 6 Calibration / Adjustment

We recommend an annual calibration and if necessary adjustment of the measuring instrument at the manufacturer.

Please observe the enclosed inspection certificate.

### 7 Inputs signals ext. sensor DP 510

|   |                  |   |
|---|------------------|---|
| Input signals   |                  |   |
| Current signal<br>(0 – 20 mA / 4 – 20 mA)<br>internal or external<br>power supply | Measuring range  | 0 – 20 mA / 4 – 20 mA   |
|   | Resolution       | 0,0001 mA   |
|   | Accuracy         | $\pm 0,03 \text{ mA} \pm 0,05 \%$   |
|   | Input resistance | 50 $\Omega$   |
| Voltage signal<br>(0 - 1V)  | Measuring range  | 0 - 1 V   |
|   | Resolution       | 0,05 mV   |
|   | Accuracy         | $\pm 0,2 \text{ mV} \pm 0,05 \%$  |
|   | Input resistance | 100 k $\Omega$  |
| Voltage signal<br>(0 - 10 V / 30 V)   | Measuring range  | 0 - 10 V/30 V   |
|   | Resolution       | 0,5 mV  |
|   | Accuracy         | $\pm 2 \text{ mV} \pm 0,05 \%$  |
|   | Input resistance | 1 M $\Omega$  |
| RTD<br>Pt100  | Measuring range  | -200 - 850 °C   |
|   | Resolution       | 0,1 °C  |
|   | Accuracy         | $\pm 0,2 \text{ °C}$ at -100 - 400 °C<br>$\pm 0,3 \text{ °C}$ (further range)   |
| RTD<br>Pt1000   | Measuring range  | -200 - 850 °C   |
|   | Resolution       | 0,1 °C  |
|   | Accuracy         | $\pm 0,2 \text{ °C}$ at -100 - 400 °C<br>$\pm 0,3 \text{ °C}$ ( further range ) |
| Pulse   | Measuring range  | minimal pulse length 100 $\mu\text{s}$<br>frequency 0 - 1 kHz<br>max. 30 VDC    |

### 8 Cable cross section

#### 8.1 Sensor circuit points/Output signal:

AWG16 – AWG28, cable cross-sections: 0,14 - 1,5 mm<sup>2</sup>

## Connection diagrams of the different sensor types (DP 510 only)

### 9 Connection diagrams of the different sensor types (DP 510 only)

#### 9.1 Connector pin assignment for all sensors DP 510

The interface connector to be used is an ODU Medi Snap 8 pin – Reference: K11M07-P08LFD0-6550


Available connection cables at CS-Instruments are:

ODU with Open ends: Order no 0553 0501, cable length: 5 m.  
Order no 0553 0502, cable length: 10 m.

ODU with M12 Connector: Order no 0553 0503, cable length: 5 m.

Extension cable (ODU/ODU): Order no 0553 0504, cable length: 10 m.

#### Connection scheme:

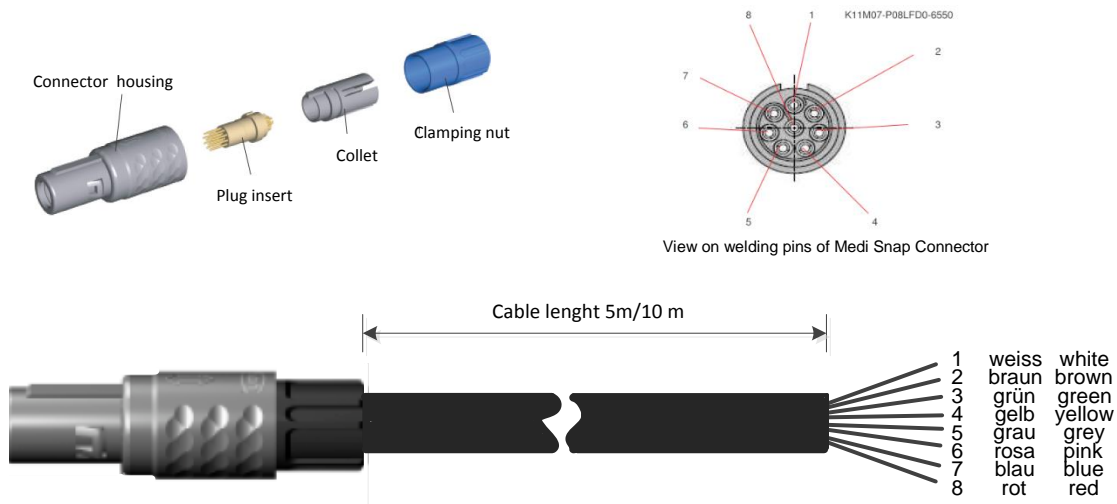


|                 |        |   |
|-----------------|--------|---|
| + RS485 ● 1     | White  | <b>+ RS485</b>  |
| - RS485 ● 2     | Brown  |   |
| SDI ● 3         | Green  | <b>SDI</b> (CS-internal Single wire Digital Interface for all dew point / Flow sensors) |
| Analog IN + ● 4 | Yellow | <b>ANALOG IN +</b>  |
| Analog IN - ● 5 | Grey   | <b>ANALOG IN -</b>  |
| I (500µA) ● 6   | Pink   | <b>STROMQUELLE 500 µA</b>   |
| +VB 24Vdc ● 7   | Blue   | <b>+VB, 24V DC Power supply for sensor</b>  |
| -VB GND ● 8     | Red    | <b>-VB, GND Sensor</b>  |

## Connection diagrams of the different sensor types (DP 510 only)


FA serial: dew point sensors from CS Instruments

VA serial: consumption sensors from CS Instruments


### 9.2 Connection CS dew point sensors series FA 415/FA 300

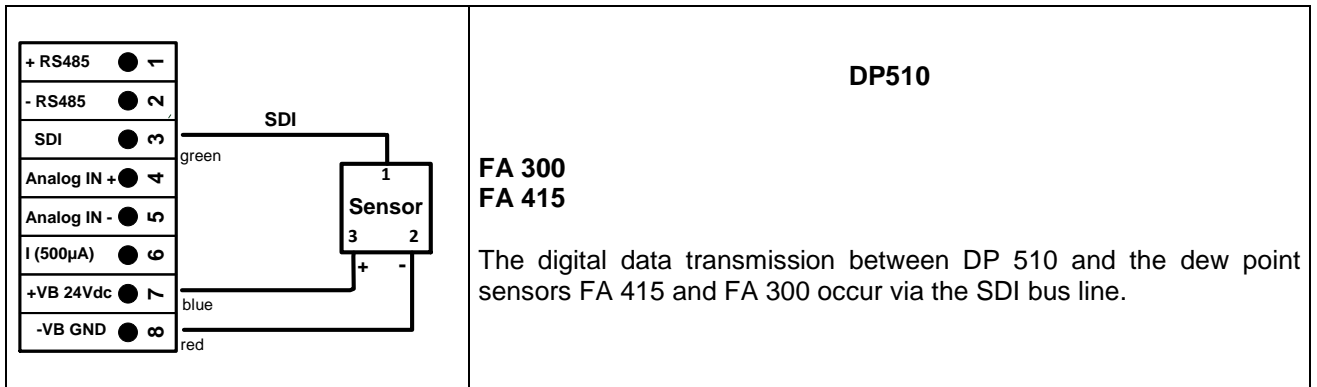

### 9.3 Connection for CS dew point- and consumption sensors, series FA/VA 400

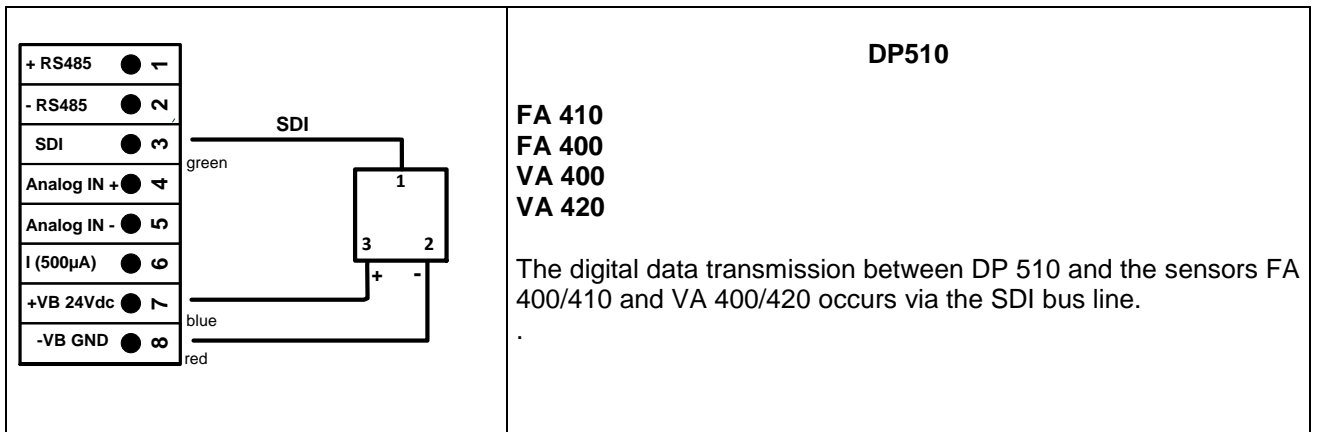

### 9.4 Connection for CS dew point- and consumption sensors, series FA/VA 5xx

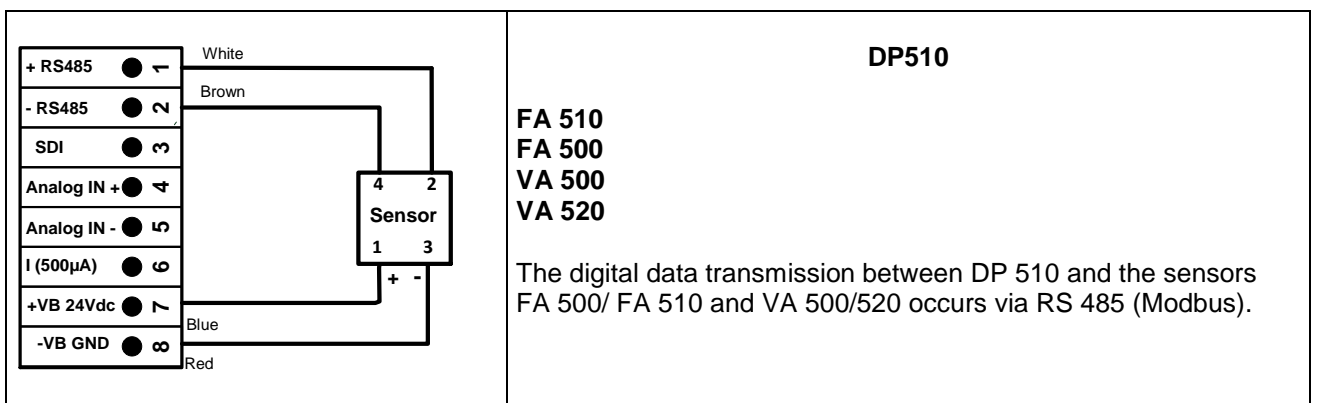




# Connection diagrams of the different sensor types (DP 510 only)

## 9.5 Connection pulse sensors

|  |  |   |
|--|--|---|
|  |  | <p>Signal level 0:<br/>low = 0 – 0,7 VDC</p> <p>Signal level 1:<br/>high = 2,5 – 30 VDC</p> <p>t = 400 µs</p> <p>max. frequency<br/>(duty cycle 1:1) = 1000 Hz</p> <p>input resistance:<br/>min. 100 kilo ohm</p> |
|  |  | <p>Required external<br/>R = 4K7</p> <p><b>Attention:</b><br/>The DP 510 is counting a consumption unit, by switching „power on“.</p>   |
|  |  | <p>Required external<br/>R = 4K7</p>  |
|  |  | <p>Not possible / allowed!</p>  |


# Connection diagrams of the different sensor types (DP 510 only)

## 9.6 Analogue two-, three-, and four-wire current signal

| Sensors with 4 - 20 mA-output in 2-wire technology  |         |   |   |         |   |   |     |   |   |             |   |   |             |   |   |           |   |   |           |   |   |         |   |   |              |
|---|---------|---|---|---------|---|---|-----|---|---|-------------|---|---|-------------|---|---|-----------|---|---|-----------|---|---|---------|---|---|--------------|
| <table border="1" style="display: inline-table; vertical-align: top;"> <tr><td>+ RS485</td><td>●</td><td>1</td></tr> <tr><td>- RS485</td><td>●</td><td>2</td></tr> <tr><td>SDI</td><td>●</td><td>3</td></tr> <tr><td>Analog IN +</td><td>●</td><td>4</td></tr> <tr><td>Analog IN -</td><td>●</td><td>5</td></tr> <tr><td>I (500µA)</td><td>●</td><td>6</td></tr> <tr><td>+VB 24Vdc</td><td>●</td><td>7</td></tr> <tr><td>-VB GND</td><td>●</td><td>8</td></tr> </table>    | + RS485 | ● | 1 | - RS485 | ● | 2 | SDI | ● | 3 | Analog IN + | ● | 4 | Analog IN - | ● | 5 | I (500µA) | ● | 6 | +VB 24Vdc | ● | 7 | -VB GND | ● | 8 | <p>DP510</p> |
| + RS485   | ●       | 1 |   |         |   |   |     |   |   |             |   |   |             |   |   |           |   |   |           |   |   |         |   |   |              |
| - RS485   | ●       | 2 |   |         |   |   |     |   |   |             |   |   |             |   |   |           |   |   |           |   |   |         |   |   |              |
| SDI   | ●       | 3 |   |         |   |   |     |   |   |             |   |   |             |   |   |           |   |   |           |   |   |         |   |   |              |
| Analog IN +   | ●       | 4 |   |         |   |   |     |   |   |             |   |   |             |   |   |           |   |   |           |   |   |         |   |   |              |
| Analog IN -   | ●       | 5 |   |         |   |   |     |   |   |             |   |   |             |   |   |           |   |   |           |   |   |         |   |   |              |
| I (500µA)   | ●       | 6 |   |         |   |   |     |   |   |             |   |   |             |   |   |           |   |   |           |   |   |         |   |   |              |
| +VB 24Vdc   | ●       | 7 |   |         |   |   |     |   |   |             |   |   |             |   |   |           |   |   |           |   |   |         |   |   |              |
| -VB GND   | ●       | 8 |   |         |   |   |     |   |   |             |   |   |             |   |   |           |   |   |           |   |   |         |   |   |              |
| Sensors with 4 - 20 mA output in 3-wire technology  |         |   |   |         |   |   |     |   |   |             |   |   |             |   |   |           |   |   |           |   |   |         |   |   |              |
| <table border="1" style="display: inline-table; vertical-align: top;"> <tr><td>+ RS485</td><td>●</td><td>1</td></tr> <tr><td>- RS485</td><td>●</td><td>2</td></tr> <tr><td>SDI</td><td>●</td><td>3</td></tr> <tr><td>Analog IN +</td><td>●</td><td>4</td></tr> <tr><td>Analog IN -</td><td>●</td><td>5</td></tr> <tr><td>I (500µA)</td><td>●</td><td>6</td></tr> <tr><td>+VB 24Vdc</td><td>●</td><td>7</td></tr> <tr><td>-VB GND</td><td>●</td><td>8</td></tr> </table>   | + RS485 | ● | 1 | - RS485 | ● | 2 | SDI | ● | 3 | Analog IN + | ● | 4 | Analog IN - | ● | 5 | I (500µA) | ● | 6 | +VB 24Vdc | ● | 7 | -VB GND | ● | 8 | <p>DP510</p> |
| + RS485   | ●       | 1 |   |         |   |   |     |   |   |             |   |   |             |   |   |           |   |   |           |   |   |         |   |   |              |
| - RS485   | ●       | 2 |   |         |   |   |     |   |   |             |   |   |             |   |   |           |   |   |           |   |   |         |   |   |              |
| SDI   | ●       | 3 |   |         |   |   |     |   |   |             |   |   |             |   |   |           |   |   |           |   |   |         |   |   |              |
| Analog IN +   | ●       | 4 |   |         |   |   |     |   |   |             |   |   |             |   |   |           |   |   |           |   |   |         |   |   |              |
| Analog IN -   | ●       | 5 |   |         |   |   |     |   |   |             |   |   |             |   |   |           |   |   |           |   |   |         |   |   |              |
| I (500µA)   | ●       | 6 |   |         |   |   |     |   |   |             |   |   |             |   |   |           |   |   |           |   |   |         |   |   |              |
| +VB 24Vdc   | ●       | 7 |   |         |   |   |     |   |   |             |   |   |             |   |   |           |   |   |           |   |   |         |   |   |              |
| -VB GND   | ●       | 8 |   |         |   |   |     |   |   |             |   |   |             |   |   |           |   |   |           |   |   |         |   |   |              |
| Sensors with 4 - 20 mA output in 4-wire technology  |         |   |   |         |   |   |     |   |   |             |   |   |             |   |   |           |   |   |           |   |   |         |   |   |              |
| <table border="1" style="display: inline-table; vertical-align: top;"> <tr><td>+ RS485</td><td>●</td><td>1</td></tr> <tr><td>- RS485</td><td>●</td><td>2</td></tr> <tr><td>SDI</td><td>●</td><td>3</td></tr> <tr><td>Analog IN +</td><td>●</td><td>4</td></tr> <tr><td>Analog IN -</td><td>●</td><td>5</td></tr> <tr><td>I (500µA)</td><td>●</td><td>6</td></tr> <tr><td>+VB 24Vdc</td><td>●</td><td>7</td></tr> <tr><td>-VB GND</td><td>●</td><td>8</td></tr> </table>  | + RS485 | ● | 1 | - RS485 | ● | 2 | SDI | ● | 3 | Analog IN + | ● | 4 | Analog IN - | ● | 5 | I (500µA) | ● | 6 | +VB 24Vdc | ● | 7 | -VB GND | ● | 8 | <p>DP510</p> |
| + RS485   | ●       | 1 |   |         |   |   |     |   |   |             |   |   |             |   |   |           |   |   |           |   |   |         |   |   |              |
| - RS485   | ●       | 2 |   |         |   |   |     |   |   |             |   |   |             |   |   |           |   |   |           |   |   |         |   |   |              |
| SDI   | ●       | 3 |   |         |   |   |     |   |   |             |   |   |             |   |   |           |   |   |           |   |   |         |   |   |              |
| Analog IN +   | ●       | 4 |   |         |   |   |     |   |   |             |   |   |             |   |   |           |   |   |           |   |   |         |   |   |              |
| Analog IN -   | ●       | 5 |   |         |   |   |     |   |   |             |   |   |             |   |   |           |   |   |           |   |   |         |   |   |              |
| I (500µA)   | ●       | 6 |   |         |   |   |     |   |   |             |   |   |             |   |   |           |   |   |           |   |   |         |   |   |              |
| +VB 24Vdc   | ●       | 7 |   |         |   |   |     |   |   |             |   |   |             |   |   |           |   |   |           |   |   |         |   |   |              |
| -VB GND   | ●       | 8 |   |         |   |   |     |   |   |             |   |   |             |   |   |           |   |   |           |   |   |         |   |   |              |

Connection diagrams of the different sensor types (DP 510 only)


9.7 Three- and four-wire power supply 0 - 1/10/30 VDC

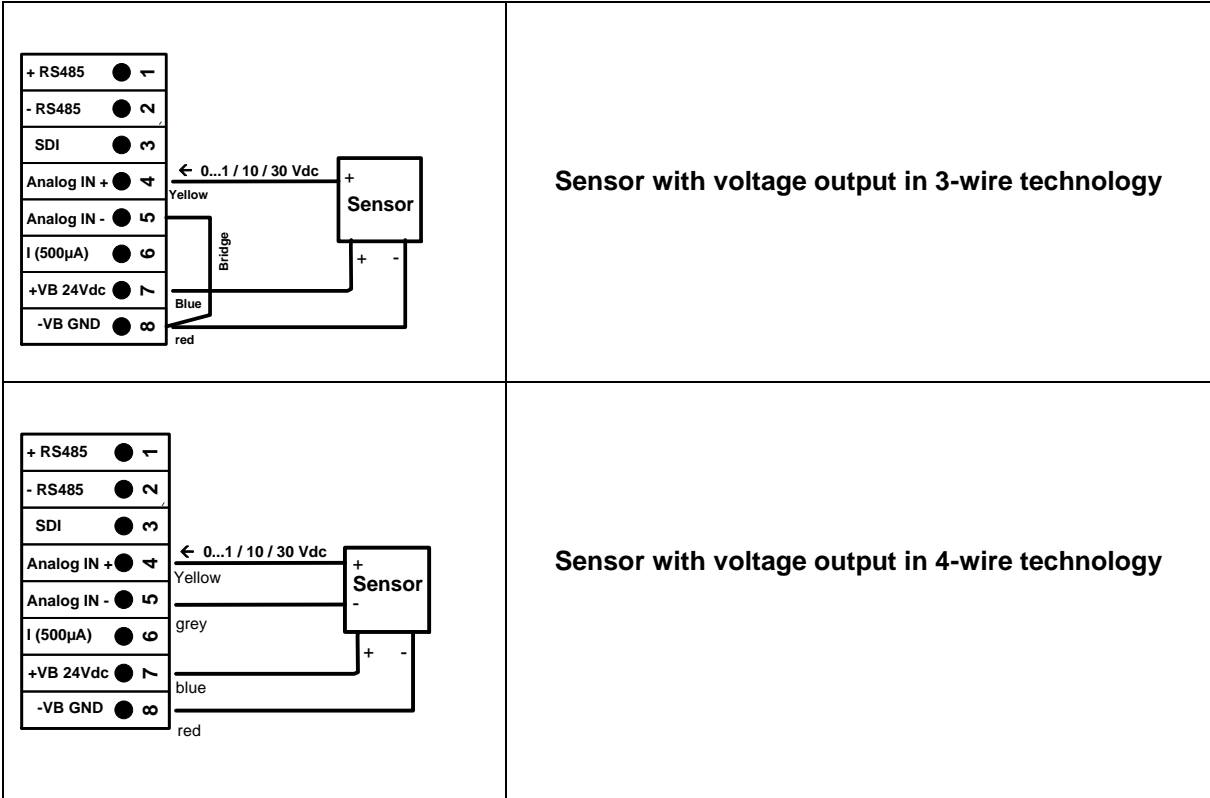




## Connection diagrams of the different sensor types (DP 510 only)

### 9.8 Two-, three-, and four-wire connector pin assignments for PT100/PT1000/KTY81

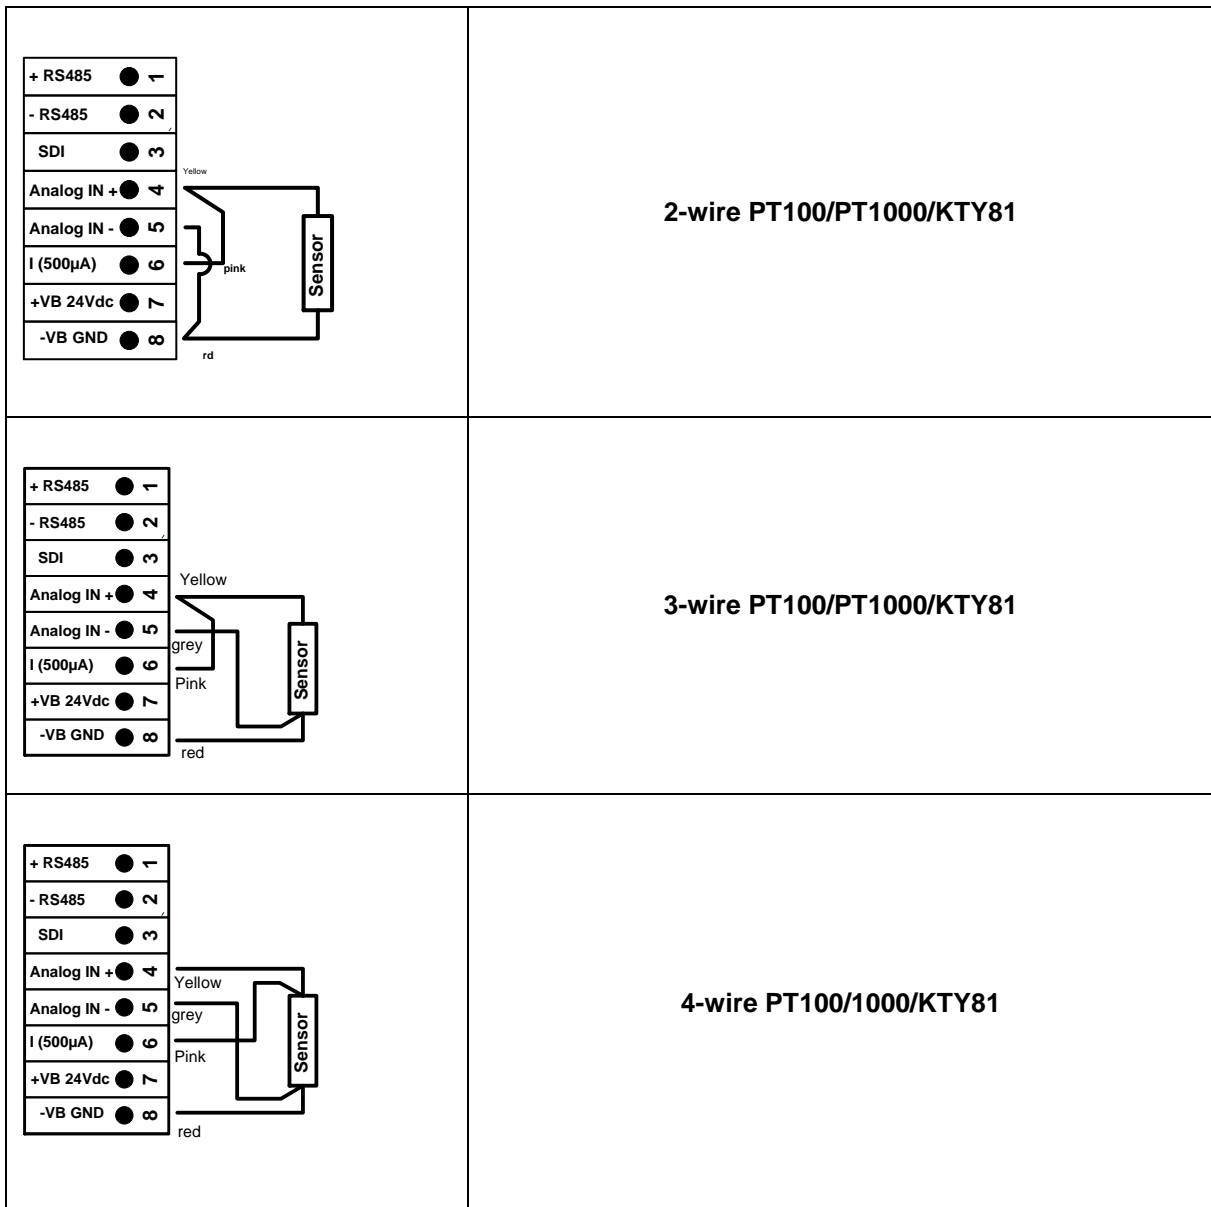

### 9.9 Connection with RS485

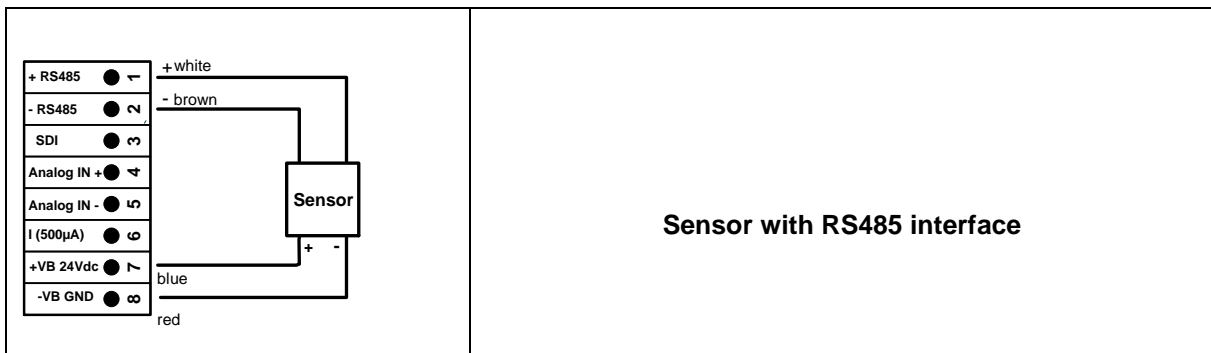


## 10 Operation DP 500 / DP 510



The operation of the DP 500 / DP 510 by means of a keypad and a touch panel

### 10.1 Keypad

#### 10.1.1 On- and Off button

On-or Off switching by long press  buttons.

#### 10.1.2 Brightness buttons



With the button  and  the display brightness can be changed.

#### 10.1.3 Screenshot-Button



By pressing the Screenshot-button, the actual display content will be stored.  
Storage is possible either to a USB Stick or on to the internal SD-card

##### 10.1.3.1 Storing Screenshot

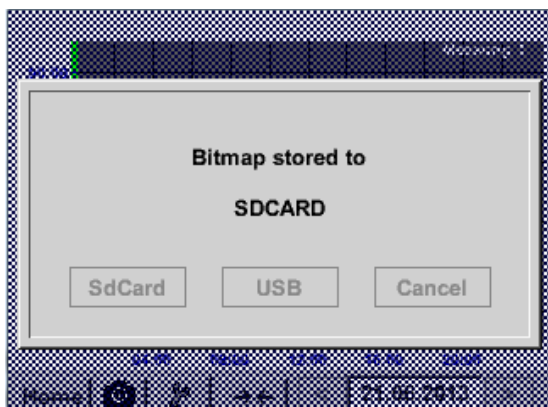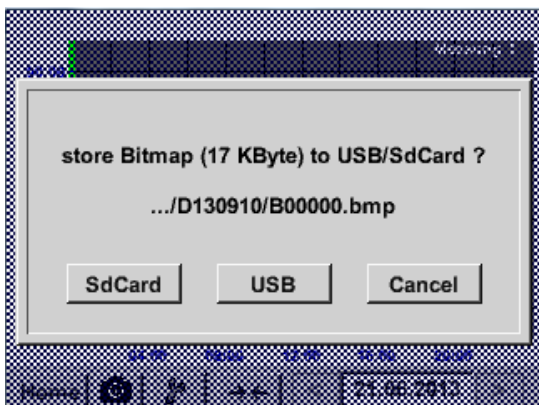

After pressing the Screenshot button a menu (see left) appears where the storage target, USB Stick or internal SD-card, could be selected.

The screens are stored as bitmap and the naming is a consecutively number. For new every day a new folder is created.

Folder definition;                   DJJMMTT  
D=fix(for date)  
JJ = year  
MM= month  
TT= day

Path: DEV0003/DP500/Bitmap

Example: first picture 10. September 2013


\\DEV0003/P500/Bitmap/D130910/B00000.bmp

# Operation DP 500 / DP 510 - Touchpanel

## 10.1.3.2 Export Screenshots


The stored bitmaps on the SD-card could be exported to a USB –Stick.

Main menu → Export/Import → Export Screenshots

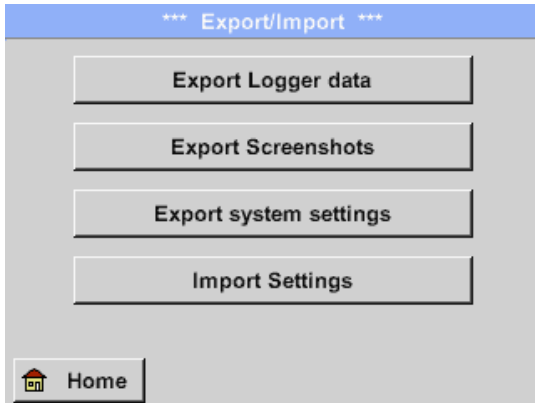

With *Export Screenshots* the stored Screenshots will be transferred to a USB-Stick.

Main menu → Export Data → Export Screenshots

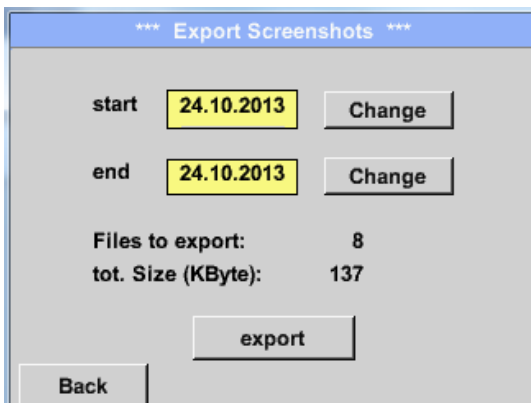

Use the *Change* buttons to adjust a period between *start* and *end*. Stored bitmaps data in this period are exported.

Main menu → Export Data → Export Screenshots → Change




The selected date is always green, and the date numbers of the Sundays are red, like in the calendar.

On days, where bitmaps were recorded, the date numbers are optical highlighted.

# Operation DP 500 / DP 510 - Touchpanel

Main menu → Export Data → Export Screenshots → Export

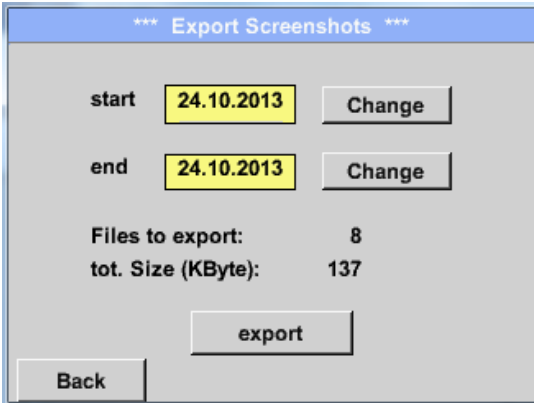

The Screenshots of the selected period are exported to the USB-Stick.

### 10.2 Touchpanel

The operation is largely self-explanatory and menu-driven via the touch panel. The selection of the respective menu items occur via short "tapping" with the finger or a soft round pen.

**Attention: Please use no pens or other objects with sharp edges!  
The foil can be damaged!**

After sensors are connected, they also have to be configured.

Inputs or changes can be made with all white deposit fields. The measured values can be represented as a curve or values.

Words in **green font** refer mainly to the pictures in the section of the chapter, but also on important menu paths or menu items that are related to are in **green font**.


The menu navigation is generally in a **green font**!

The table of contents and chapter references in **blue font** contain links to the respective chapter title.

## 10.3 Main menu (Home)

From the main menu, you can reach every available item.

### 10.3.1 Initialization

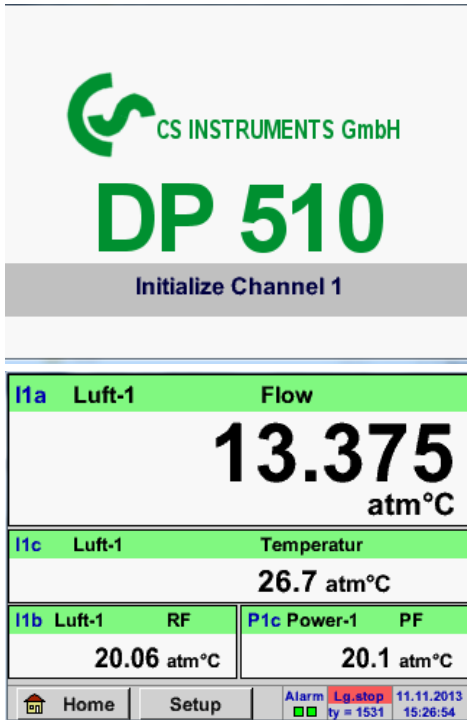

After switching on the DP500 / DP510 all channels are initialized and the menu „ *Real time values* „ appears.


**Attention:**  
For the first initiation, there may be no external channel for DP 510 preset!

Please see chapter [10.3.2.1.2 Sensor Settings](#) then select appropriate configurations and set!

# Main menu

## 10.3.2 Main menu

Home

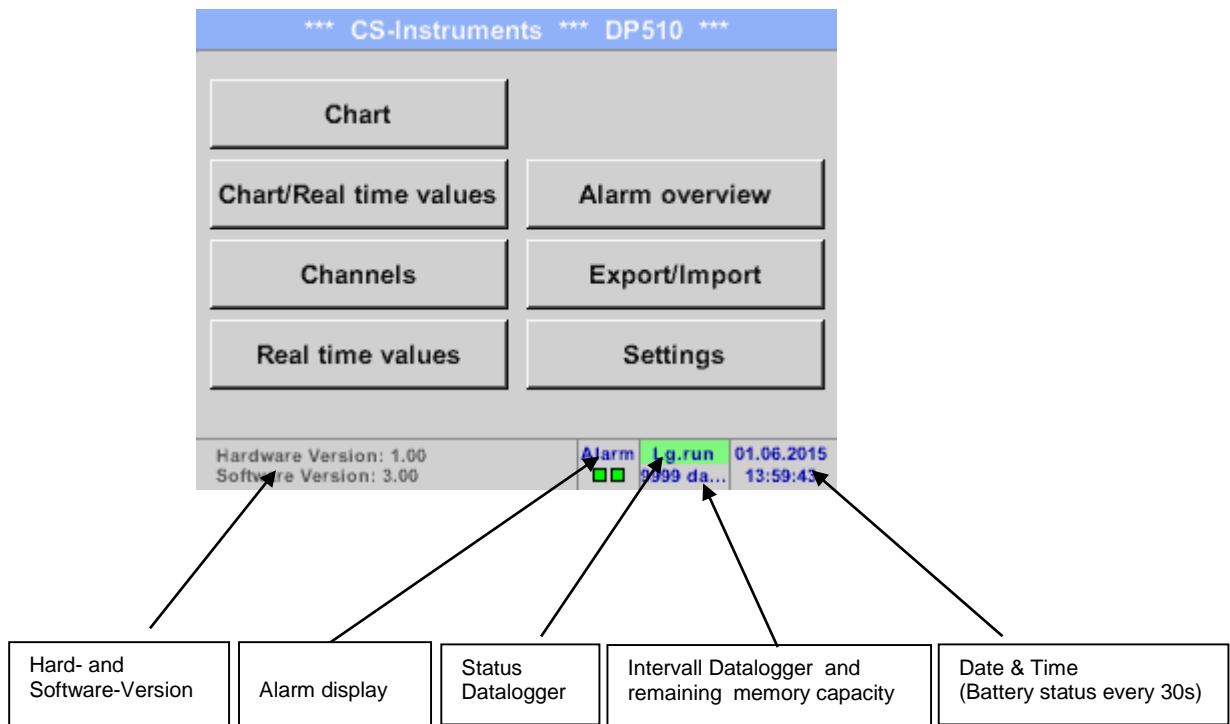

### **Important:**

Before the first sensor setting is made, the language and time should be set!

### **Remark:**

Chapter [10.3.2.1.3.1 language](#)

*Main → Settings → Device Settings → Set Language)*

Chapter [10.3.2.1.3.2 Date & Time](#)

*Main → Settings → Device Settings → Date & Time)*

## Settings / Password-Settings

### 10.3.2.1 Settings



The settings are all protected by a password!

Settings or changes are generally confirmed with **OK!**

**Remark:**


If you go back to main menu and then again one of the setting menus is called, you must enter the password again.

Main menu → Settings

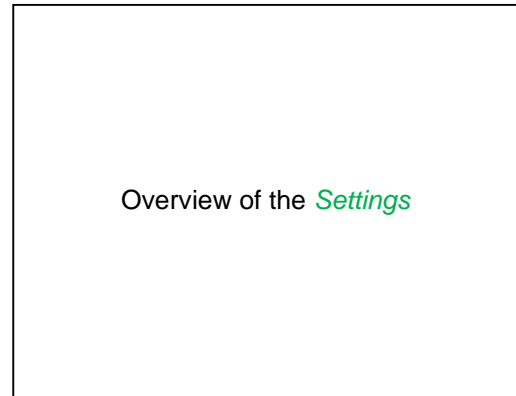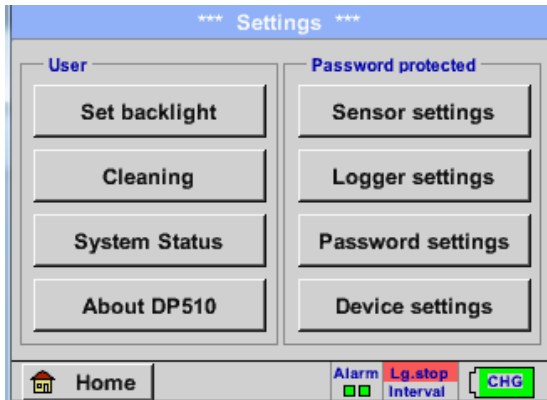

#### 10.3.2.1.1 Password-Settings


Main menu → Settings → Password settings

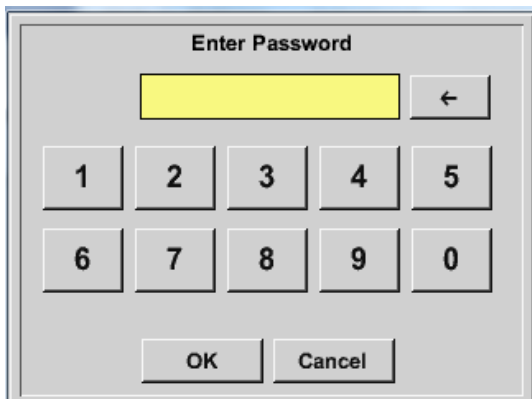

Factory settings for password at the time of delivery: 0000 (4 times zero).

If required, the password can be changed in the *Password settings*.

The new password must be entered two times in a row and in each case confirmed with **OK**

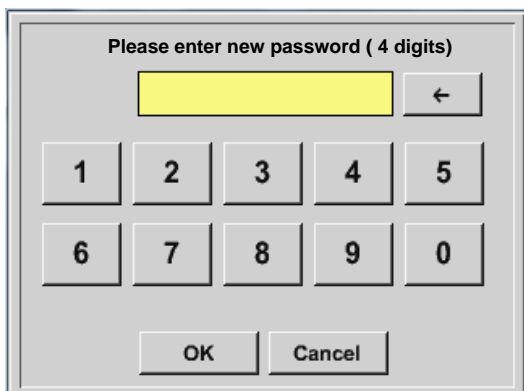

If an incorrect password is entered there appears *Enter password* or *New password repeat* in red font.

If you cannot remember the password, please use Master password in order to enter a new password.

**Remark:**

The master password is supplied together with the instrument's documentation.




# Sensor-Settings - Naming the measurement data

## 10.3.2.1.2 Sensor-settings

### Important:

Sensors from CS Instruments are generally pre-configured and can be connected directly to an external sensor channel! (DP 510 only)


Main menu → Settings → Sensor settings

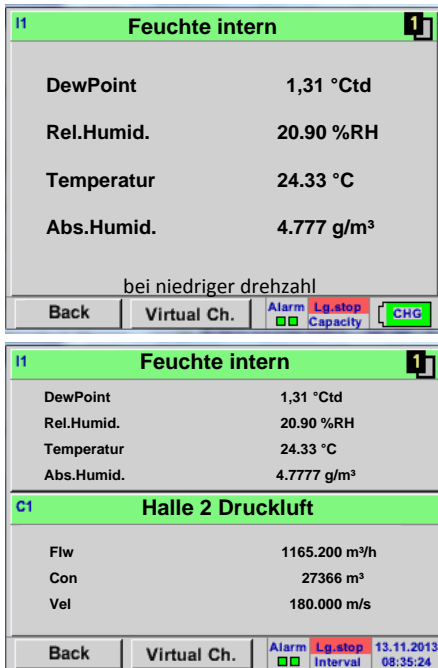

An overview of the available channels appears after entering the password. Depending on the version DP 500 or DP 510 without or with the external sensor channel.

**Remark:**  
Usually there is no preset for the external channel!

Main menu → Settings → Sensor settings → I1 → arrow right (2.page)

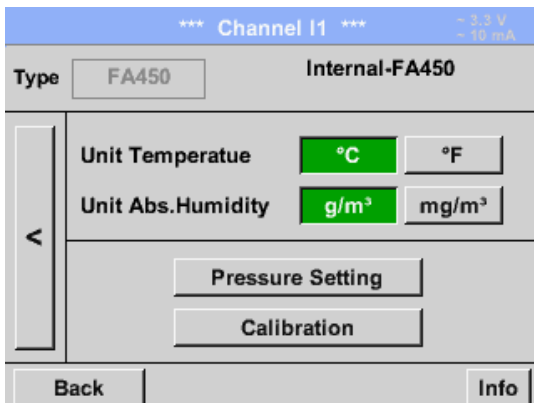

In the upper block it the units for the temperature, °C and °F, as well as for the absolute humidity, g/m³ and mg/m³, can be selected.

## Main menu

### 10.3.2.1.2.1 Settings internal Dew point-Sensor

With the DP 500/510 the pressure dew point in the pressure line is measured automatically. The pressure dew point is always related to the pressure in the line.

A pressure input is not necessary, because the measuring principle measures independent of pressure.

The DP 500/510 is able simultaneously to the pressure dew point also calculate the atmospheric dew point or dew point at reduced pressure.


For the calculation of the atmospheric dew point (if the gas would be expanded to ambient pressure) or the dew point at reduced pressure, it is necessary to define the reference pressure and the system pressure.

#### 10.3.2.1.2.1.1 Definition of the System pressure (relative pressure value)

Actual there are 2 possibilities to define system pressure (input as relative pressure value)

- System pressure as a fixed value
- System pressure taken over from an external pressure sensor ( only DP 510)



Main menu → Settings → Sensor settings → I1 → arrow right (2.page) → Pressure Setting → Fixed

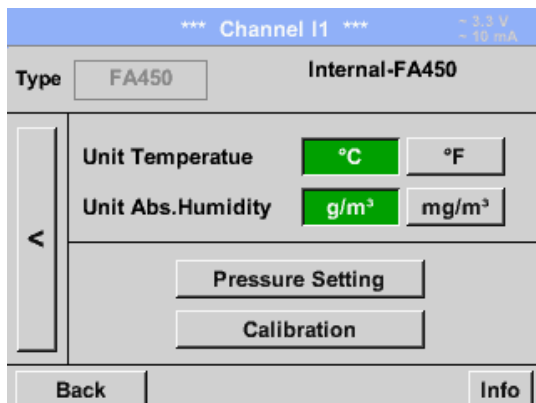

By activating the button *fixed* the value of the system pressure could be inserted in the corresponding text field.

Pressure unit is freely selectable. Selection menu is opened by pressing the button corresponding units

Confirm the settings by pressing the *OK* button.

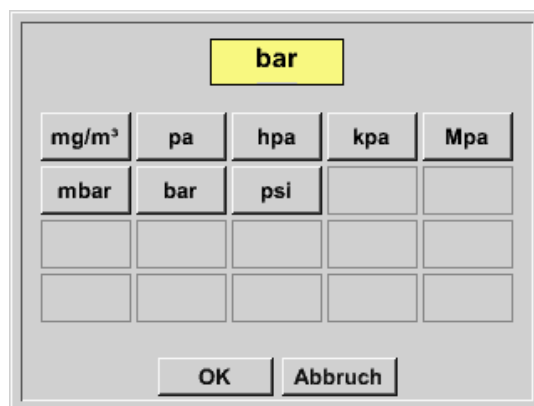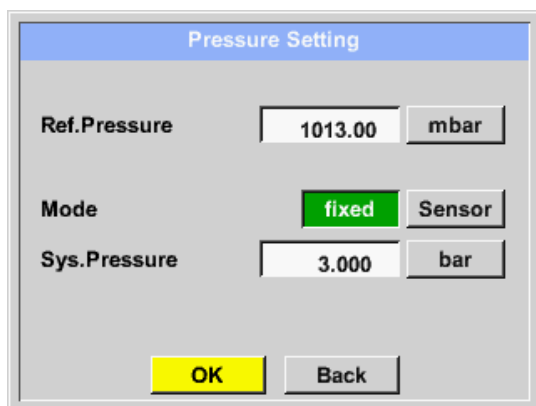

## Main menu

Main menu → Settings → Sensor settings → I1 → arrow right (2.page) → Pressure Setting → Sensor

Pressure Setting

Ref.Pressure 1013.00 mbar

Mode fixed **Sensor**

Sys.Pressure C1a (C1a) bar

OK Back

When using an ext. Pressure probe on sensor input C1 (only DP 510) then the **Sensor** button have to be activated.

By entering the System pressure text field the possible channels and the relevant values could be selected.

Only values with pressure units are selectable.

Confirm the settings by pressing the **OK** button.

Select Channel & Value

I1 **C1 (a)** P1

V1 V2

OK Cancel

Select Value

**C1a C1a (bar)** C1b min (bar)

C1c max (bar) C1d Gesamt (mA)

C1e -- (°C) C1f -- ()

C1g -- (User\_1) C1h -- (cts/m³)

Back

### 10.3.2.1.2.1.2 Definition of Reference pressure (absolute pressure value)

Main menu → Settings → Sensor settings → I1 → arrow right (2.page) → Pressure Setting → Text field Ref.Pressure

Pressure Setting

Ref.Pressure 1013.00 mbar

Mode **fixed** Sensor

Sys.Pressure 3.000 bar

OK Back

Reference pressure is the pressure for that the dew point in relaxation will be back-calculated.

Default- Value is 1013 mbar (Atm. Pressure).

Confirm the settings by pressing the **OK** button.

## Main menu

### 10.3.2.1.2.2 Choice of the sensor type (For example type CS-Digital sensor)


Main menu → Settings → Sensor settings → C1



If still no sensor has been configured, the *Type No Sensor* appears.

By pushing the description field *Type No Sensor* the list of sensor types appears (see next step).


Main menu → Settings → Sensor settings → C1 → Type description field → CS-Digital

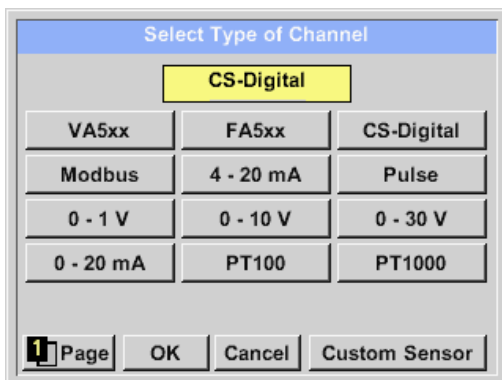

Now the *Type CS-Digital* is selected for the VA/FA 400 series and confirmed by pressing the *OK* button.

### 10.3.2.1.2.3 Label and setting the description fields

Main menu → Settings → Sensor settings → C1 → Text filed Name

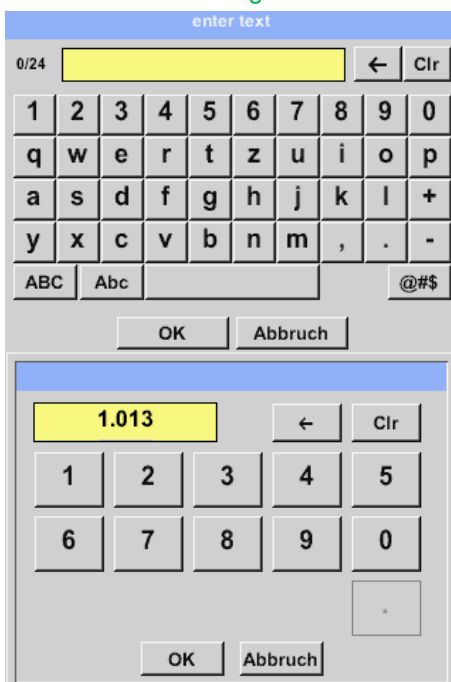

In the case of text description field, a menu opens with the corresponding selection

- For name fields, a keyboard as you can see left side.
- For value fields a keypad as you can see left
- In case of a selection field a corresponding menu with possible entries will be displayed. See therefore chapter Sensor settings.

For the sensor name, it is possible to enter a name with up to 24 characters. For values names are max. 10 characters and for the short name max. 3 characters possible.

## Main menu

### 10.3.2.1.2.4 Name the measurement data and define the decimal places


#### Remark:

The *Resolution* of the decimal places, the *Short Name* and *Value Name* are found under the **Tool button!**



**Tool Button:**

Main menu → Settings → Sensor settings → C1 → Tool Button

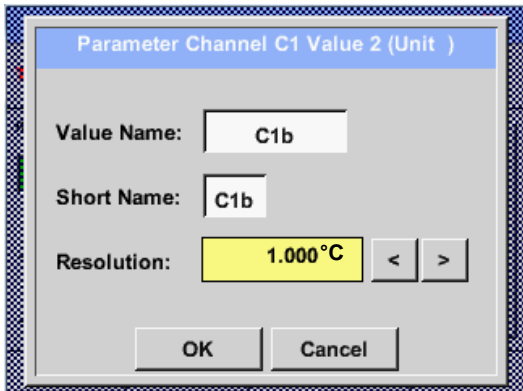


For the recorded *Value* there can be entered a *Name* with 10 characters and later in menu item *Graphics/Real time values* it is easier to identify it. Otherwise the *Name* is, for example, **C1b**. The channel name is **C1** and *a* is the first measurement data at the channel, the Second *b* and the Third *c*. The *Resolution* of the decimal places is simply adjustable by pushing right and left (0 to 5 decimal places).

See chapter 10.3.2.1.2.3 label and setting the description fields

### 10.3.2.1.2.5 Recording measurement data

Main menu → Settings → Sensor settings → C1 → Record Button

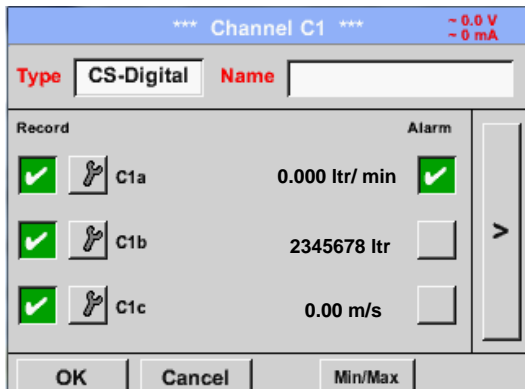

Use the *Record* buttons to select the measurement data that will be stored by **activated data logger**.

#### Attention:

Before the selected measurement data are recorded, the data logger must be activated after the settings (See chapter 12.3.2.5.5 *Logger-Settings(Datalogger)*).

## Sensor-Settings / Alarm-Settings

### 10.3.2.1.2.6 Alarm-Settings ( Alarm Popup)

Main menu → Settings → Sensor settings → C1 → → Alarm-Button

By pushing an alarm button, the following window appears:

In the alarm settings, an *Alarm 1* and *Alarm 2* incl. *Hysteresis* can be entered for each channel.

In the menu *Alarm overview* (can be reached from the main menu), the alarm settings are clearly represented.

Main menu → Settings → Sensor settings → C1 → → Alarm-Button → Alarm-1- und Alarm-2-buttons + Popup-buttons

Here for example the *Alarm-1* yellow and the *Alarm-2* red.

Main menu → Settings → Sensor settings → C1

After alarm setting for Channel C1a.

#### Remark:

After confirm with *OK*, the font is black again and the values and settings are accepted

## Sensor-Settings / More Settings( scale analogue output)

### 10.3.2.1.2.7 More Settings (scale analogue output)

Main menu → Settings → Sensor settings → A1 → arrow right (2.page) → More settings

More-Settings C1-Luft-1

4...20mA Output of Sensor  
Base

m<sup>3</sup>/h m/s

scale manual

4mA = 0.000 m/s

20mA = -1.#|0 m/s

Max Velocity 92.700 m/s

Calibration Data

Gas Air (287.0)

Temperat 293.0 °K

Pressure 1000.0 hPa

Area 110.0 mm<sup>2</sup>

Cal. Date 24.07.2013

OK Cancel

In *More-Settings*, you can define whether the 4 - 20 mA analogue output of the sensor based on the flow rate or velocity.

The green highlighted description field is selected!

In addition, you can push the *scale manual* button and set the measuring range.

After confirming with *OK*, the settings are assumed.

**Remark:**  
*More-Settings* only for type **CS-Digital** available!

More-Settings C1-

4...20mA Output of Sensor  
Base

m<sup>3</sup>/h m/s

scale manual

4mA = 0.000 m/s

20mA = 200.000 m/s

Max Velocity 92.700 m/s

Calibration Data

Gas Air (287.0)

Temperat 293.00 °K

Pressure 1000.00 hPa

Area 110.00 mm<sup>2</sup>

Cal. Date 03.07.2013

OK Cancel

The settings are completed after pressing the *OK* button!

**Remark:**

After confirming with *OK*, the font is black again and the values and settings are accepted.

## Sensor-Settings / CS Digital


### 10.3.2.2 Dew Point Sensor FA 400 / FA 410 of type CS-Digital (SDI Bus)

**First step:** choose an unused sensor channel


Main menu → Settings → Sensor settings → C1

**Second step:** choose type CS-Digital

Main menu → Settings → Sensor settings → C1 → Type description field → CS-Digital

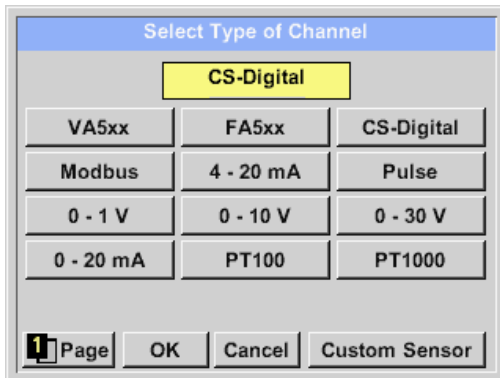


Now the *Type CS-Digital* is selected for the VA/FA 400 series and confirmed by pressing the *OK* button.

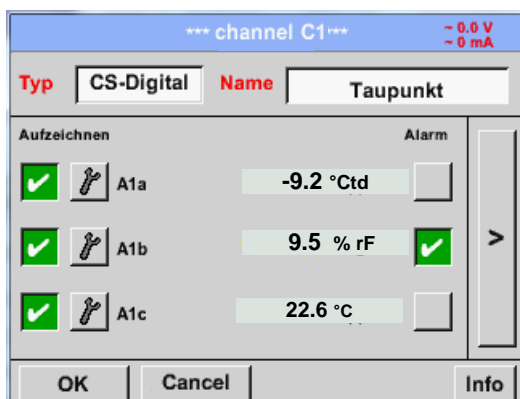

The DP 510 detects, if the connected sensor is a flow or dew point sensor of **CS Instruments** and set the *CS-Digital* subtype automatically correct.

Now, a *Name* (see Chapter 10.3.2.1.2.3 label and setting the description files), the **alarm settings** (see Chapter 10.3.2.1.2.5 Alarm-Settings) and the **recording-settings** (see Chapter 10.3.2.1.2.4 Recording measurement data) and the *Resolution* of the decimal places (see Chapter 10.3.2.1.2.3 Name measurement data and define the decimal places) can be determined.

Main menu → Settings → Sensor settings → C1 → Name description field

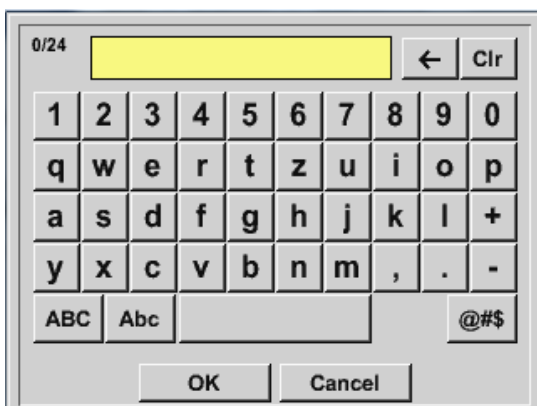

It is possible to enter a name with 24 characters.

**Third step:** confirm with *OK* two times



## Sensor-Settings / Typ FA 5xx

### 10.3.2.3 Flow sensor VA 400 / VA 420 of type CS-Digital (SDI Bus)

**First step:** choose an unused sensor settings channel  
Main menu → Settings → Sensor settings → C1

**Second step:** choose type CS-Digital  
Main menu → Settings → Sensor settings → C1 → Type description field → CS-Digital

| Select Type of Channel |           |            |               |
|------------------------|-----------|------------|---------------|
| CS-Digital             |           |            |               |
| VA5xx                  | FA5xx     | CS-Digital |               |
| Modbus                 | 4 - 20 mA | Pulse      |               |
| 0 - 1 V                | 0 - 10 V  | 0 - 30 V   |               |
| 0 - 20 mA              | PT100     | PT1000     |               |
| Page                   | OK        | Cancel     | Custom Sensor |

Now the *Type CS-Digital* is selected for the VA/FA 400 series and confirmed by pressing the *OK* button.

\*\*\* Channel C1 \*\*\* ~ 24.8 V  
~ 53 mA

Type CS-Digital Name Consumption

| Record  | Alarm                    |
|---|--------------------------|
| <input checked="" type="checkbox"/> C1a 0.00 m³/h | <input type="checkbox"/> |
| <input checked="" type="checkbox"/> C1b 4444 m³   | <input type="checkbox"/> |
| <input checked="" type="checkbox"/> C1c 0.00 m/s  | <input type="checkbox"/> |

Back Store Min/Max

Das DP 510 erkennt, ob es sich bei dem angeschlossenen Sensor um ein Durchfluss- oder Taupunkt-Sensor von **CS Instruments** handelt und stellt den **CS-Digital** Subtyp automatisch richtig ein.

Now, a *Name* (see Chapter 10.3.2.1.2.3 label and setting the description files), the **alarm settings** (see Chapter 10.3.2.1.2.5 Alarm-Settings) and the **recording-settings** (see Chapter 10.3.2.1.2.4 Recording measurement data) and the *Resolution* of the decimal places (see Chapter 10.3.2.1.2.3 Name measurement data and define the decimal places) can be determined.

Main menu → Settings → Sensor settings → C1 → Name description field

0/24 Consumption ← Clr

|     |     |   |   |   |   |   |   |    |    |
|-----|-----|---|---|---|---|---|---|----|----|
| 1   | 2   | 3 | 4 | 5 | 6 | 7 | 8 | 9  | 0  |
| q   | w   | e | r | t | z | u | i | o  | p  |
| a   | s   | d | f | g | h | j | k | l  | +  |
| y   | x   | c | v | b | n | m | , | .  | -  |
| ABC | Abc |   |   |   |   |   |   | @# | \$ |


OK Cancel

It is possible to enter a name with 24 characters.

**Third step:** confirm with *OK* two times

## Sensor-Settings / CS Digital

Main menu → Settings → Sensor settings → C1 → arrow right (2.page)

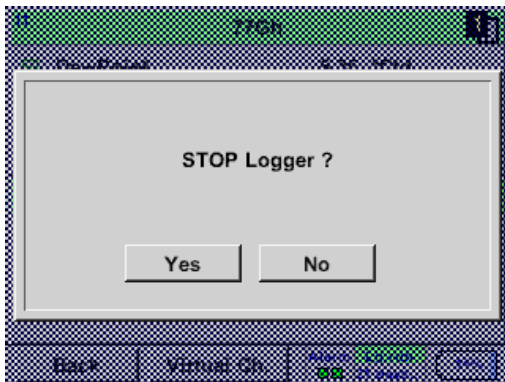



If the data logger is activated, the following window will appear and via pushing **Yes** it can be disabled.

*(Only activated, if already settings and recordings are made)*

**Remark:**


If sensor settings are defined or changed, the data logger must be stopped.

Main menu → Settings → Sensor settings → C1 → arrow right (2.page) → diameter description field

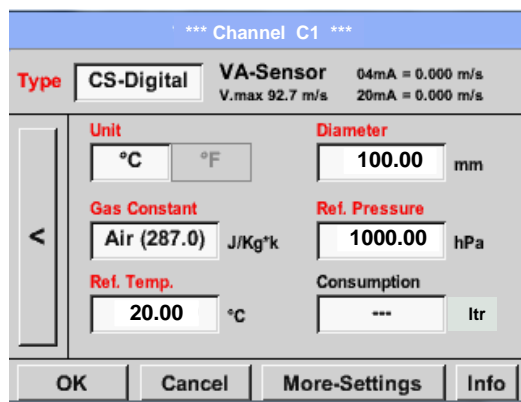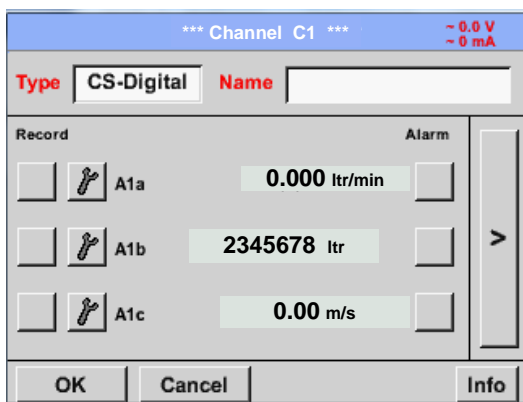

By entering the white text fields the value could be added or changed content could be change

Main menu → Settings → Sensor settings → C1 → arrow right (2.page) → diameter description field

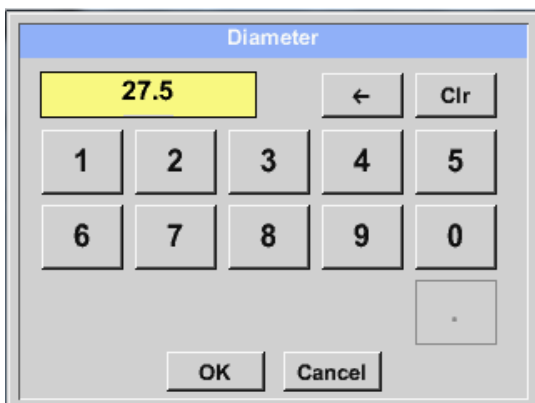

**Important:**

The **inner diameter** of flow tube can be entered here, if this was not automatically correctly set.

Here the **inner diameter** was set to 27.5mm.

Please confirm by pressing the **OK** button and go back with **arrow left (1.page)**.


**Important:**

The **inner diameter** should be entered as precisely as possible, because otherwise the measurement results are not correct!

There is no uniform standard for the tube **inner diameter**!  
(Please, inquire at the manufacturer or measure by your own!)


## Sensor-Settings / CS Digital

Main menu → Settings → Sensor settings → C1 → arrow right (2.page) → Text field Unit

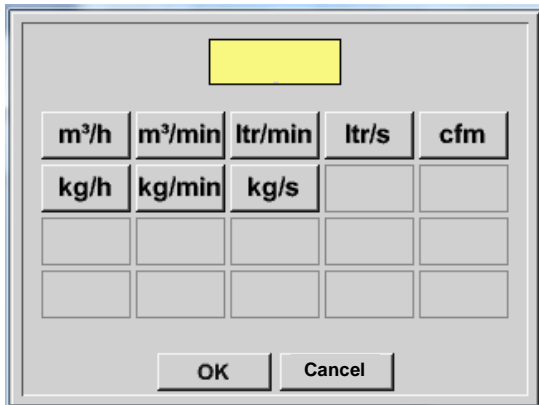

A preset selection of suitable *Units*.

Main menu → Settings → Sensor settings → C1 → arrow right (2.page) → Gas Constant description field

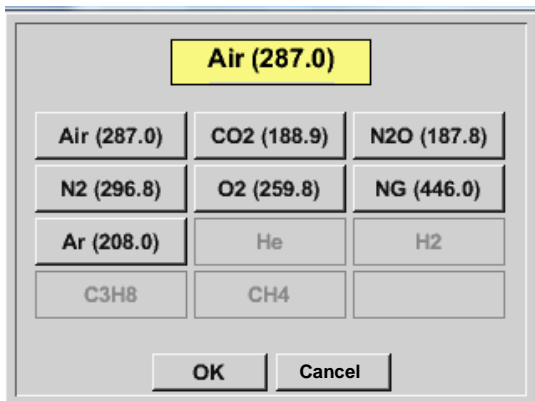

A preset selection of suitable *Gas Constants*.

### Remark:

After confirm with **OK**, the font is black again and the values and settings are accepted.

### Attention:

**Reference temperature and reference pressure (factory setting 20 °C, 1000 hPa):**  
All volume flow values (m³/h) and consumption values indicated in the display are related to 20 °C, 1000 hPa (according to ISO 1217 intake condition)  
0 °C and 1013 hPa (= standard cubic meter) can also be entered as a reference.  
Do not enter the operation pressure or the operation temperature under reference conditions!

# Sensor-Settings / Typ FA 5xx


## 10.3.2.4 Dew Point Sensor FA 500 / FA 510 of type FA 5xx (RS 485 Modbus)

**First step:** choose an unused sensor digital channel

Main menu → Settings → Sensor settings → C1

**Second step:** choose type FA 5xx)


Main menu → Settings → Sensor settings → C1 → Type description field → FA 5xx

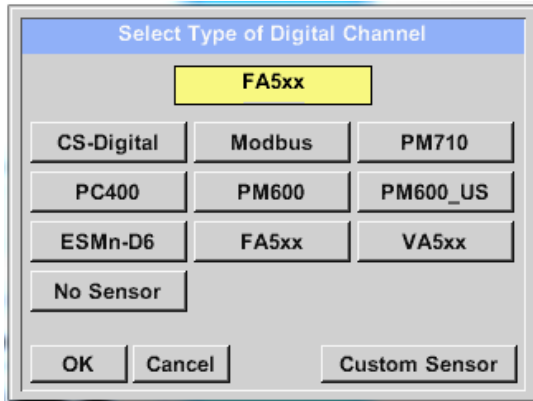

Now the *Type FA 5xx* is selected for the FA 5xx series and confirmed by pressing the *OK* button.

Now, a *Name* (see Chapter 10.3.2.1.2.3 label and setting the description files), the *alarm settings* (see Chapter 10.3.2.1.2.5 Alarm-Settings) and the *recording-settings* (see Chapter 10.3.2.1.2.4 Recording measurement data) and the *Resolution* of the decimal places (see Chapter 10.3.2.1.2.3 Name measurement data and define the decimal places) can be determined.



Main menu → Settings → Sensor settings → C1 → text description field Name

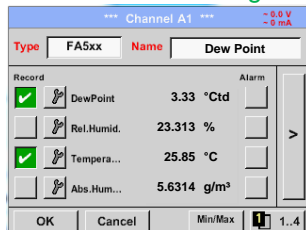

Input of a name, please enter the text field „Name“.

It is possible to enter a name with max. 24 characters.

Confirmation by pressing the *OK*-button.

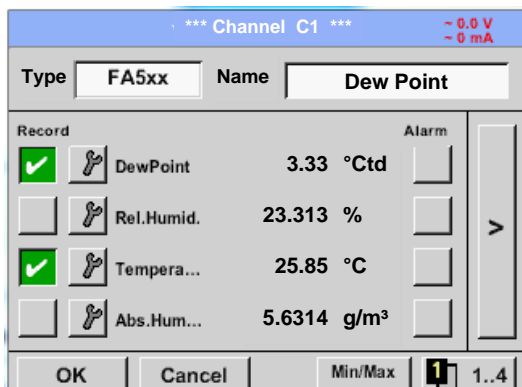


The connection with the FA 5xx sensor is done after confirmation by pressing “*OK*”.

## 10.3.2.4.1 Settings Dew point sensor FA 500 FA 510

### 10.3.2.4.1.1 Unit selection for temperature and humidity

Main menu → Settings → Sensor settings → A1 → arrow right (2.page)

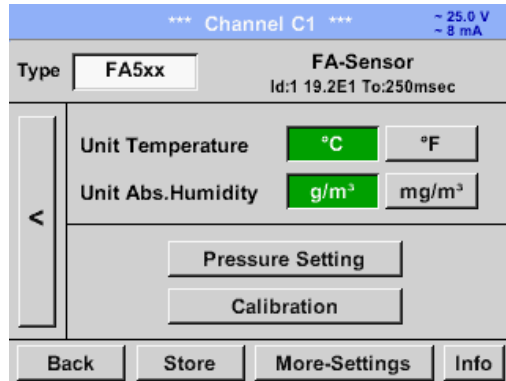

Unit selection for temperature and humidity by pressing the button °C, °F, g/m³ or mg/m³.


Confirm the settings by pressing the OK button.

### 10.3.2.4.1.2 Definition of the System pressure (relative pressure value)

Actual there are 2 possibilities to define system pressure (input as relative pressure value)

- System pressure as a fixed value
- System pressure taken over from an external pressure sensor


Main menu → Settings → Sensor settings → C1 → arrow right (2.page) → Pressure Setting → Fixed

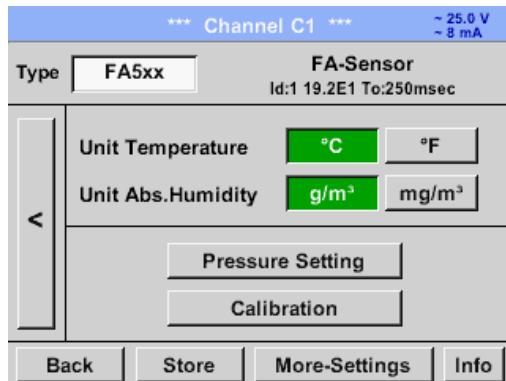

The definition of the fixed value system pressure value is done by activating the button "fixed", but this is only required in case a ext. pressure probe is connected.


The value is entered in the corresponding text field. The unit can be freely selected, selection menu is opened by pressing the corresponding button units

Confirm the settings by pressing the OK button.

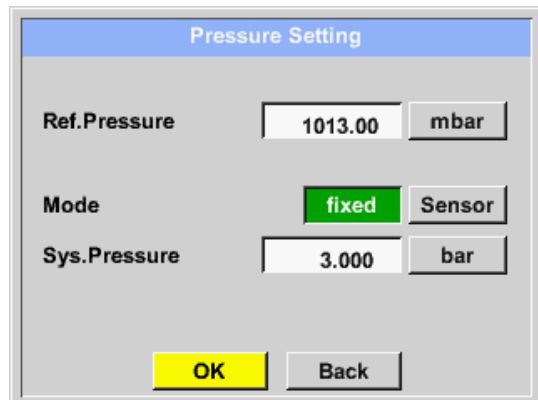

### 10.3.2.4.1.3 Definition of Reference pressure (absolute pressure value)

Main menu → Settings → Sensor settings → C1 → arrow right (2.page) → Pressure Setting → Text field Ref.Pressure

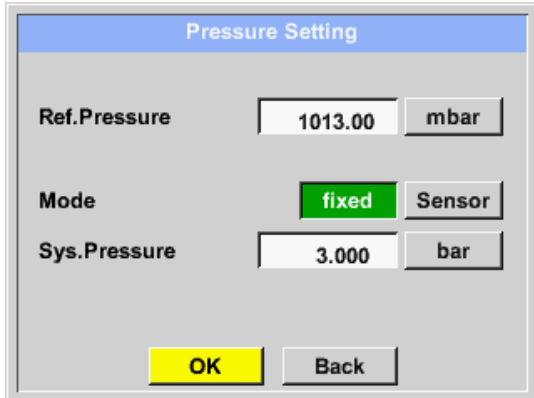


Reference pressure is the pressure for that the dew point in relaxation will be back-calculated.

Default- Value is 1013 mbar (Atm. Pressure).

Confirm the settings by pressing the **OK** button.


### 10.3.2.4.2 Calibration

Main menu → Settings → Sensor settings → C1 → arrow right (2.page) → Calibration

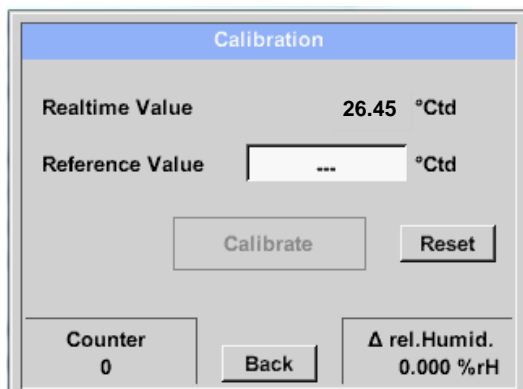

Here, a one-point calibration can be performed.

For that purpose, please enter in the text box "**Reference Value**" the new correct dew point value.

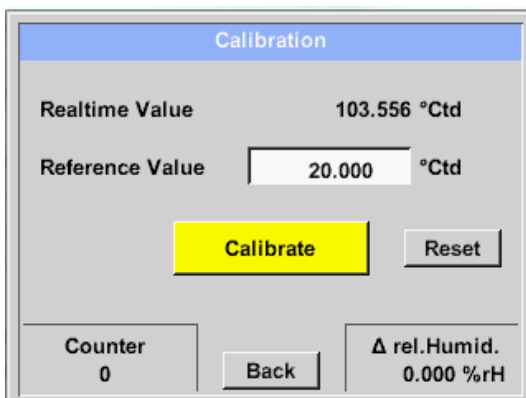

Then by pressing the "Calibration" button taking over the inserted reference value.

Calibration can be put back to factory setting by pressing "**Reset**".

For each performed calibration, the counter is increased by 1.

### 10.3.2.4.3 More Settings Analogue output 4-20mA

Main menu → Settings → Sensor settings → C1 → arrow right (2.page) → More-Settings → 4-20mA

| 4-20mA Settings |          |           |        |        |
|-----------------|----------|-----------|--------|--------|
| None            | Temp °C  | Temp °F   | rH     | DP °C  |
| DP °F           | AbsHu(g) | AbsHu(mg) | HumGrd | VapRat |
| SatVapPr        | ParVapPr | ADP °C    | ADP °F |        |

4mA =  °C

20mA =  °C

ErrorVal.

This menu allows the adjustment / assignment of the measurement value and the scaling of the analogue output.

Selection of the measurement value by selecting the appropriate measured value key in this example, "DP °C" for dew point ° Ctd.

In text fields "4mA" and "20mA" the appropriate scaling values are entered, here from -80 ° Ctd (4mA) to -20 ° Ctd (20mA).

With "Error Val" is determined what is output in case of error at the analog output.

- <3.6 Sensor error / System error
- 22 Sensor error / System error
- 4..20 Output according Namur (3.8mA – 20.5 mA)  
< 4mA to 3.8 mA Measuring range under range  
>20mA to 20.5 mA Measuring range exceeding

## Sensor - Settings / Type VA 5xx


### 10.3.2.5 Flow sensor of type VA 5xx (RS 485 Modbus)

**First step:** choose an unused sensor digital channel

Main menu → Settings → Sensor settings → C!


**Second step:** choose type VA 5xx

Main menu → Settings → Sensor settings → C1 → Type description field → VA 5xx

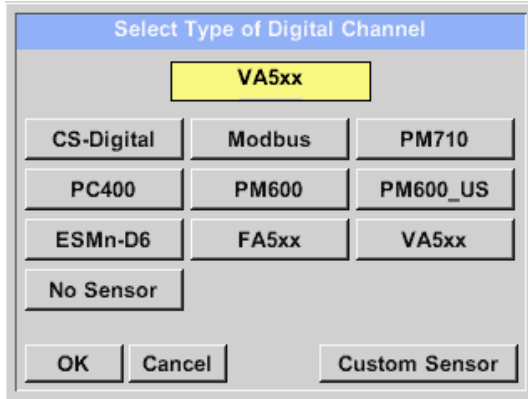

Now the *Type VA 5xx* is selected for the VA 5xx series and confirmed by pressing the **OK** button.


Now, a *Name* (see Chapter 10.3.2.1.2.3 label and setting the description files), the **alarm settings** (see Chapter 10.3.2.1.2.5 Alarm-Settings) and the **recording-settings** (see Chapter 10.3.2.1.2.4 Recording measurement data) and the *Resolution* of the decimal places (see Chapter 10.3.2.1.2.3 Name measurement data and define the decimal places) can be determined.

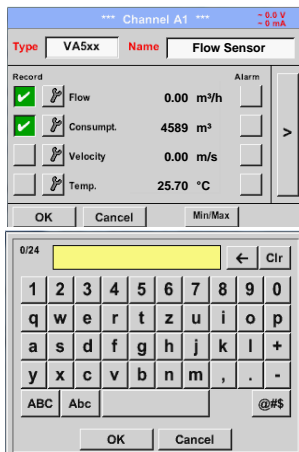

Input of a name, please enter the text field *„Name“*.

It is possible to enter a name with max. 24 characters.

Confirmation by pressing the **OK**-button.

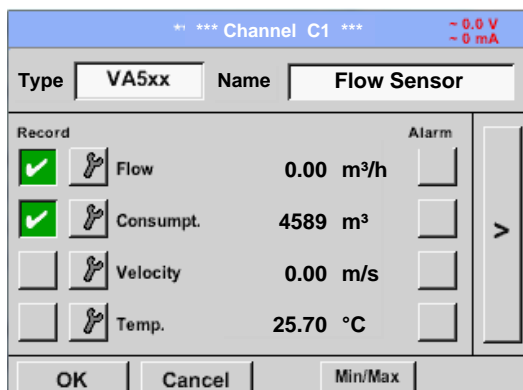

The connection with the VA 5xx sensor is done after confirmation by pressing **“OK”**.



## Sensor - Settings / VA 5xx

### 10.3.2.5.1 Settings for Flow sensor VA 5xx

Main menu → Settings → Sensor settings → C1 → arrow right (2.page)

| *** Channel C1 *** |               | ~ 0.0 V       |      |
|--------------------|---------------|---------------|------|
|                    |               | ~ 0 mA        |      |
| Type               | VA5xx         | VA-Sensor     |      |
| Flow               | Velocity      | Diameter      | Unit |
| m³/h               | m/s           | 53.100        | mm   |
| Gas Constant       | Ref. Pressure | Unit          |      |
| Air (real) J/Kg*k  | 1000.00       | mbar          |      |
| Ref. Temp.         | Unit          | Count.Val     | Unit |
| 20.000             | °C            | 4589          | m³   |
| OK                 | Cancel        | More-Settings | Info |

For each text field could be the either a value or a unit be set.

Settings by entering the text field and then input a value or select the unit for the appropriate field.

In case of VA 520 and VA 570 with integrated measuring section the diameter and diameter unit field are not access able.

#### 10.3.2.5.1.1 Diameter settings

Main menu → Settings → Sensor settings → C1 → arrow right (2.page) → diameter description field

| Diameter |   |        |     |   |
|----------|---|--------|-----|---|
| 27.5     |   | ←      | Clr |   |
| 1        | 2 | 3      | 4   | 5 |
| 6        | 7 | 8      | 9   | 0 |
| .        |   |        |     |   |
| OK       |   | Cancel |     |   |

#### **Important:**

The **inner diameter** of flow tube can be entered here, if this was not automatically correctly set.

In

Please confirm by pressing the **OK** button and go back with **arrow left (1.page)**.

#### **Important:**

The **inner diameter** should be entered as precisely as possible, because otherwise the measurement results are not correct!

There is no uniform standard for the tube **inner diameter**!  
(Please, inquire at the manufacturer or measure by your own!)

## Sensor - Settings / VA 5xx

### 10.3.2.5.1.2 Gas Constant settings

Main menu → Settings → Sensor settings → C1 → arrow right (2.page) → Gas Constant description field

| Air (real) |             |             |
|------------|-------------|-------------|
| Air (real) | CO2 (real)  | H2 (real)   |
| NO2 (real) | CO2 (188.9) | N2O (187.8) |
| N2 (296.8) | O2 (259.8)  | NG (446.0)  |
| Ar (208.0) |             |             |

OK Cancel

All gases marked in blue and with (real) have been a real gas calibration curve stored in the sensor.

Select the gas you require and confirm selection by pressing **OK** button.

#### **Attention:**

**Reference temperature and reference pressure (factory setting 20 °C, 1000 hPa):**  
All volume flow values (m<sup>3</sup>/h) and consumption values indicated in the display are related to 20 °C, 1000 hPa (according to ISO 1217 intake condition)  
0 °C and 1013 hPa (= standard cubic meter) can also be entered as a reference.  
Do not enter the operation pressure or the operation temperature under reference conditions!

## Sensor - Settings / VA 5xx

### 10.3.2.5.1.3 Definition of the reference conditions

Here, the desired measured media reference conditions for pressure and temperature can be defined

Main menu → Settings → Sensor settings → C1 → arrow right (2.page) → Ref. Pressure description field  
 Main menu → Settings → Sensor settings → C1 → arrow right (2.page) → Ref. Pressure Unit description field

The left screenshot shows the 'Ref. Pressure' input screen. A yellow box highlights the value '1000'. Below it is a numeric keypad with buttons for digits 1-9, 0, and a decimal point. There are also back and clear (Clr) buttons. At the bottom are 'OK' and 'Cancel' buttons.

The right screenshot shows the unit selection screen. A yellow box highlights 'mbar'. Below it is a grid of unit options: mbar, psi, hpa, and several empty boxes. At the bottom are 'OK' and 'Cancel' buttons.

Main menu → Settings → Sensor settings → C1 → arrow right (2.page) → Ref. Temp. description Field  
 Main menu → Settings → Sensor settings → C1 → arrow right (2.page) → Ref. Temp. Unit description Field

The left screenshot shows the 'Ref. Temp.' input screen. A yellow box highlights the value '20'. Below it is a numeric keypad with buttons for digits 1-9, 0, and a decimal point. There are also back and clear (Clr) buttons. At the bottom are 'OK' and 'Cancel' buttons.

The right screenshot shows the unit selection screen. A yellow box highlights '°C'. Below it is a grid of unit options: °C, °F, and several empty boxes. At the bottom are 'OK' and 'Cancel' buttons.

### 10.3.2.5.1.4 Definition Unit of flow and velocity

Main menu → Settings → Sensor settings → C1 → arrow right (2.page) → Flow description Field  
 Main menu → Settings → Sensor settings → C1 → arrow right (2.page) → Velocity description Field

The left screenshot shows the flow unit selection screen. A yellow box highlights 'm³/h'. Below it is a grid of various flow units: m³/h, Nm³/h, m³/min, Nm³/min, ltr/h, Nltr/h, ltr/min, Nl/min, ltr/s, Nl/s, cfm, SCFM, kg/h, kg/min, kg/s, and kW. At the bottom are 'OK' and 'Cancel' buttons.

The right screenshot shows the velocity unit selection screen. A yellow box highlights 'm/s'. Below it is a grid of various velocity units: m/s, Nm/s, fpm, SFPM, and several empty boxes. At the bottom are 'OK' and 'Cancel' buttons.

### 10.3.2.5.1.5 Definition consumption counter value and consumption unit

## Sensor - Settings / VA 5xx

Main menu → Settings → Sensor settings → C1 → arrow right (2.page) → Count Val. description Field  
 Main menu → Settings → Sensor settings → C1 → arrow right (2.page) → Count Val. Unit description Field

The sensor allows taking over a starting counter value. Inserting the value by entering the "Count. Val." text field.

In the Count. Val. Unit field different units could be used. Selection by activation of the "Count. Val. Unit" text field

In case the counter value unit will be changed only the consumption counter value will be recalculated to the appropriate unit.

Selection to confirm selection by pressing **OK** button.




**Important!**  
 When the counter reach 10000000 m<sup>3</sup> the counter will be reset to zero.

**Remark:**

After confirmation with **OK**, the font is black again and the values and settings are accepted

### 10.3.2.5.2 Settings analogue output 4-20mA of VA 5xx

Main menu → Settings → Sensor settings → C1 → More-Settings → 4-20mA Ch1

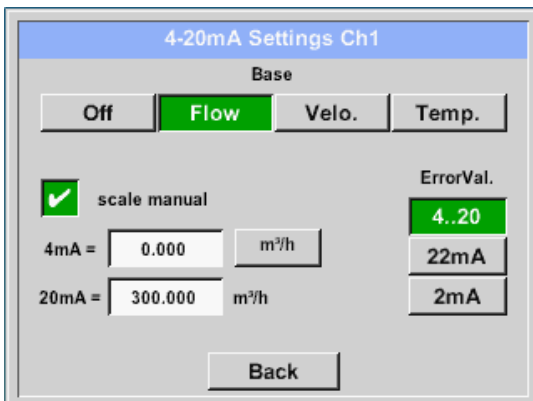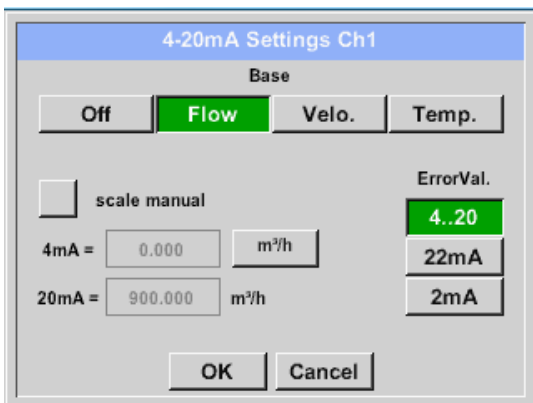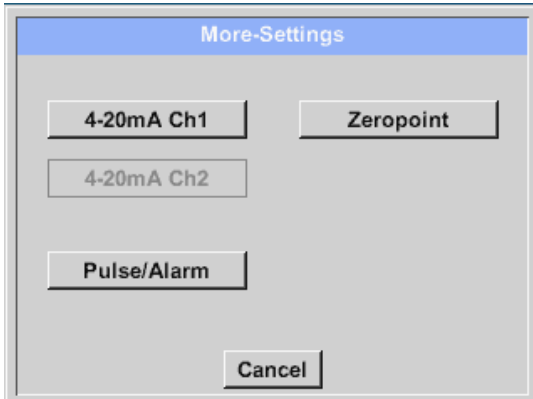

This menu allows the adjustment / assignment of the measurement value and the scaling of the analogue output by pressing the "4-20mA Ch1" button.

Selection of the analogue output measurement value by activating the appropriate measured value key in this example, "Flow".

Possible outputs are flow, velocity and temperature. In case of no use, please select "Off".

The analogue output scaling have to possibilities, automatic scaling (default) and a manual scaling by the user. Auto scaling is based on the calibration settings, means 4mA is set to zero and the 20mA value is based on the max. settings here 900m³/h

A "manual scaling" needs an activation of the "scale manual" button.

In text fields "4mA" and "20mA" the appropriate scaling values are entered, here from zero m³/h (4mA) to 300 m³/h (20mA).

With "Error Val" it is determined what is the output in case of an error at the analogue output.


- 2 mA Sensor Error / System Error
- 22 mA Sensor Error / System Error
- 4..20 Output according Namur (3.8mA – 20.5 mA)  
< 4mA to 3.8 mA Measuring range under range  
>20mA to 20.5 mA Measuring range exceeding

Inputs / changes to be confirmed with "OK" button. Return to main menu with "Back".

## Sensor - Settings / VA 5xx

### 10.3.2.5.3 Settings Pulse / Alarm output of VA 5xx

Main menu → Settings → Sensor settings → C1 → More-Settings → Pulse / Alarm

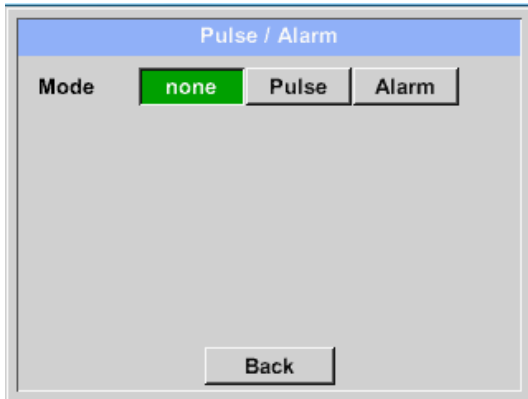


The pulse output of the VA 5xx could be set functionally as pulse output or alarm output.

Function to activate by pressing either the "Pulse" or "Alarm" button.

In case of no use, please select "none".

Inputs / changes to be confirmed with "OK" button. Return to main menu with "Back".

Main menu → Settings → Sensor settings → C1 → More-Settings → Pulse

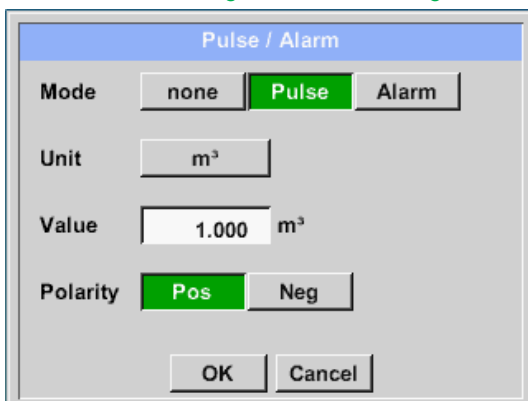

To set up the pulse first the unit and the measurement value have to be defined.


Unit selection by pressing "unit" button and choice one of the possible units "kg", "cf", "ltr" or "m³".

Pulse weight setting by entering the text field "Value".


Here with defined 1 pulse per m³ and with positive polarity.

With "Polarity" the switching state could be defined.


Pos. = 0 → 1 neg. 1 → 0



Inputs / changes to be confirmed with "OK" button. Return to main menu with "Back".

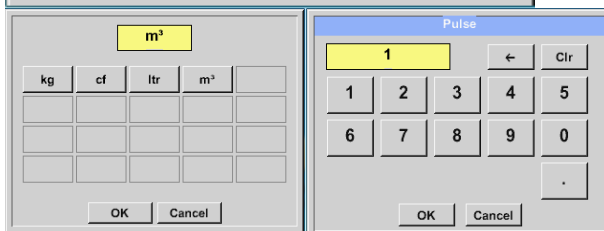

Main menu → Settings → Sensor settings → C1 → More-Settings → Alarm

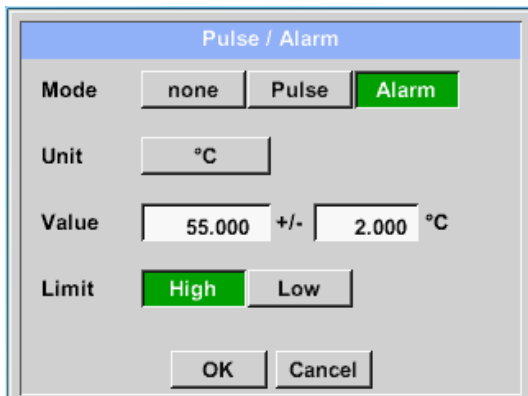

In case of use the pulse output as alarm following definitions needs to be set:


Unit selection by pressing "unit" button and choice one of the possible units "cfm", "ltr/s", "m³/h", "m/s", "°F", "°C", "kg/s" or "kg/min".

Alarm value setting by entering the text fields "Value".

The limits "High" or "Low" defines when the alarm is activated, selecting by pressing the appropriate button

**High:** Value over limit  
**Low:** Value under limit

Inputs / changes to be confirmed with "OK" button. Return to main menu with "Back".

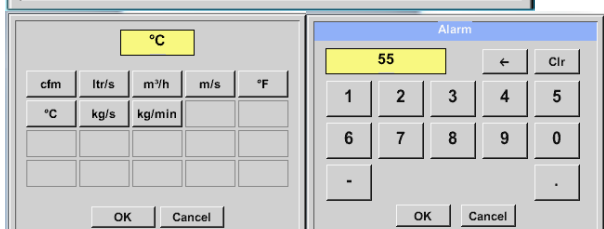

## Sensor - Settings / VA 5xx

### 10.3.2.5.4 Settings ZeroPoint or Low Flow Cut off for VA 5xx

Main menu → Settings → Sensor settings → C1 → More-Settings → Zeropoint

Zero Setup

Actual Flow 2.045

ZeroPoint

CutOff

Reset

Back

Zero Setup

Actual Flow 200.732

ZeroPoint

CutOff

Reset

OK Cancel

Zero Setup

Actual Flow 2.045

ZeroPoint

CutOff

Reset

OK Cancel

With these function following adjustments for the sensor VA 5xx could be done:

#### Zeropoint:

When, without flow, the installed sensor shows already a flow value of  $> 0 \text{ m}^3/\text{h}$  herewith the zero point of the characteristic could be reset

#### Cutoff:

With the low-flow cut off activated, the flow below the defined "LowFlow Cut off" value will be displayed as  $0 \text{ m}^3/\text{h}$  and not added to the consumption counter.

For Zero Point the text field "ZeroPoint" to enter and insert the displayed actual flow, here 2.045

For inserting low flow cutoff value activate the text field "CutOff" and insert the required value, here 10.

With the "Reset" button all entries could be set back to zero.

Inputs / changes to be confirmed with "OK" button. Return to main menu with "Back".

# Sensor-Settings / Configuration of Analogue Sensors

## 10.3.2.5.4.1 Configuration of Analog-Sensors

Applicable only at DP 510.

A brief overview of the possible *Type* of settings with examples.


For *CS-Digital* see chapter [10.3.2.1.2.2 Choice of the sensor type \(For example type CS-Digital sensor\)](#) and [10.3.2.1.2.7 Dew Point sensor with type CS-Digital](#).

The *Alarm-settings*, *Record-Button*, the *Resolution* of the decimal places and *Short Name* and *Value-Name* are all described in Chapter [10.3.2.1.2 Sensor-Settings](#).

The caption of description fields, see chapter [10.3.2.1.2.8 Label and setting the description fields!](#)

## 10.3.2.5.4.2 Type 0 - 1/10/30 Volt and 0/4 – 20 mA


Main menu → Settings → Sensor settings → C1 → Type description field → 0 - 1/10/30 V

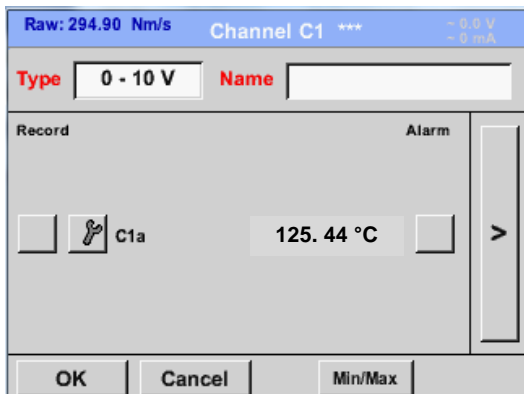

Please see the scale of the sensor (here for example *Type 0 - 10V* corresponds to 0 - 250 °C) from the data sheet of the connected sensor.

By *Scale 0V* enter the lower and by *Scale 10V* the upper scale value.


Main menu → Settings → Sensor settings → C1 → arrow right (2.page)

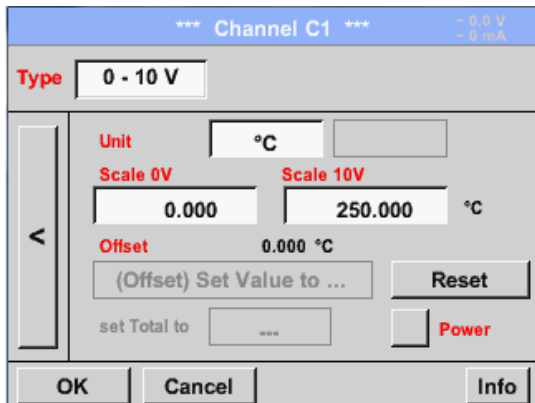

By *Scale 0V* enter the lower and by *Scale 10V* the upper scale value

The *Sensor Supply Voltage* is switched on, if it's required by the sensor type, otherwise off (no green hook).

Please confirm by pressing the *OK* button

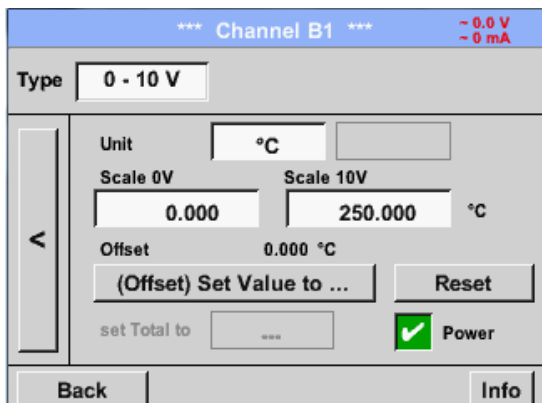

It is possible to define a Offset-Value. With the *Set Value to*-button (*Offset*) you enter it. The positive or negative difference of the *Offset* will be displayed.

By pressing the *Reset*-button the *Offset* will be deleted



## Sensor-Settings / Configuration of Analogue sensors

Main menu → Settings → Sensor settings → C1 → arrow right (2.page) → description field Unit

A preset selection of suitable units by **Type**  
*0 - 1/10/30 V and 0/4...20 mA.*

The different pages could be displayed by pressing the **Page**-button.

In addition, **User** specific units could be defined

Here with the **Edit** button could analog to **description field** a User unit be defined.

Main menu → Settings → Sensor settings → C1 → Type description field → 0/4 - 20 mA

Here for example **Type 4 - 20 mA.**

## Sensor-Settings / Configuration of Analogue sensors

### 10.3.2.5.4.3 Type PT100x and KTY81

Main menu → Settings → Sensor settings → B1 → Type description field → PT100x

\*\*\* Channel C1 \*\*\* -0.5 V  
-0 mA

Type **PT100** Name **Measure 2**

Record Alarm

B1a 123.54 °C

R

U

OK Cancel Info

Here the sensor type *PT100* and the *Unit* in °C are chosen, alternatively the sensor types *PT1000* and *KTY81*, as well as the *Unit* °F can be selected.

\*\*\* Channel C1 \*\*\* -0.5 V  
-0 mA

Type **PT100**

Unit **°C**

Sensortype: **PT100** PT1000 KTY81

Offset 0.00 °C

(Offset) Set Temp. to ... Reset

Back Info

More setting options, see chapter [10.3.2.1.2.10 Type 0 - 1/10/30 Volt and 0/4 - 20 mA!](#)

## Sensor-Settings / Configuration of Analogue sensors

### 10.3.2.5.4.4 Type Pulse (Pulse ration)

Main menu → Settings → Sensor settings → B1 → Type description field → Pulse

| Record                                  | Alarm     |
|---|-----------|
| <input checked="" type="checkbox"/> B1a | 9000 m³/h |
| <input checked="" type="checkbox"/> B1b | 367001 m³ |
| <input type="checkbox"/> B1c            | 50 Hz     |

Typically the value with unit of **1 Pulse** is standing on the sensor and can directly entered to the **1 Pulse =** description field.

**Remark:**

Here, all description fields are already labeled or occupied.

1 Pulse = 0.005 m³

| Unit | Pulse | Consumption | Counter |
|------|-------|-------------|---------|
|      | m³    | m³/h        | m³      |

Counter: 367001 m³  Power

Main menu → Settings → Sensor settings → B1 → arrow right (2.page) → Unit Pulses

|    |     |    |      |     |
|----|-----|----|------|-----|
|    | ltr | m³ | Nltr | Nm³ |
| cf | Ncf | kg | kWh  | PCS |
|    |     |    |      |     |
|    |     |    |      |     |

By *Unit Pulse* you can choose between a flow volume or a power consumption unit.

## Sensor-Settings / Configuration of Analogue sensors

Main menu → Settings → Sensor settings → B1 → arrow right (2.page) → Unit Consumption




The screenshot shows a configuration window with a grid of buttons. The top button is 'm³/h' and is highlighted in yellow. Below it are buttons for 'm³/h' and 'm³/min'. At the bottom are 'OK' and 'Cancel' buttons.

Unit of current *Consumption* by *Type Pulse*

**Remark:**  
Example with the unit cubic meters / hour

Main menu → Settings → Sensor settings → B1 → arrow right (2.page) → Unit Counter

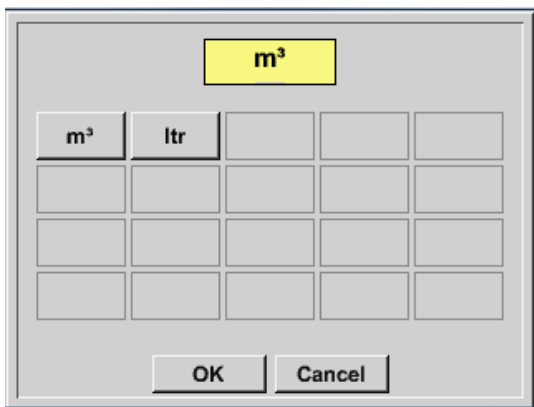

The screenshot shows a configuration window with a grid of buttons. The top button is 'm³' and is highlighted in yellow. Below it are buttons for 'm³' and 'ltr'. At the bottom are 'OK' and 'Cancel' buttons.

The available Units for the *Unit of Counter* by *Type Pulse*

The **counter** can be set any time to any value you need.


More setting options, see chapter [10.3.2.1.2.10 Type 0 - 1/10/30 Volt](#) and [0/4 - 20 mA!](#)

### 10.3.2.5.4.5 Type „No Sensor“

Main menu → Settings → Sensor settings → C1 → Type description field → No Sensor



Is used to declare a not currently needed channel as *No Sensor* defined.

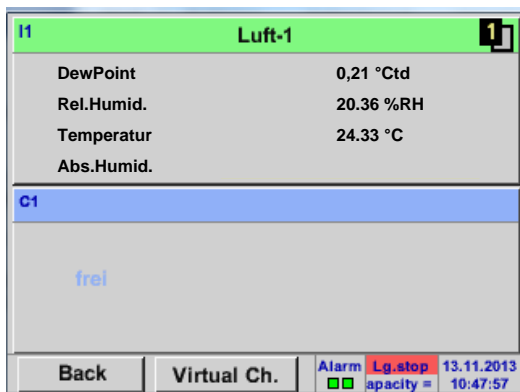

If you go to *Type No Sensor* Back, the channel will appear as *unused*.

### 10.3.2.5.4.6 Type Modbus

#### 10.3.2.5.4.7 Selection and activation of Sensor-Type Modbus

**First Step: First step:** choose an unused sensor channel

Main menu → Settings → Sensor settings → C1


**Second step:** choose type Modbus

Main menu → Settings → Sensor settings → C1 → Type description field → Modbus

**Third step:** confirm with *OK*.

Now, a **Name** (see chapter 10.3.2.1.2.8 Label and setting the description fields) can be determined.

Main menu → Settings → Sensor settings → C1 → arrow right (2.page) → Va → use

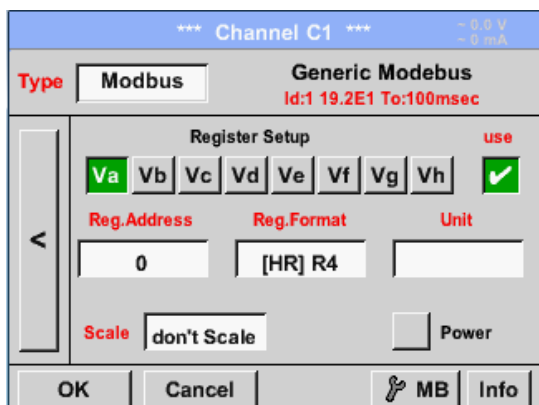


Via Modbus, it is possible to read out up to 8 Register-Values (from Input or Holding Register) of the sensor.

Selection by the Register Tabs *Va – Vh* and activation by pressing of the corresponding *Use* button.

#### 10.3.2.5.4.7.1 Modbus Settings

Main menu → Settings → Sensor settings → C1 → arrow right (2.page) → Modbus Settings → ID -Text field

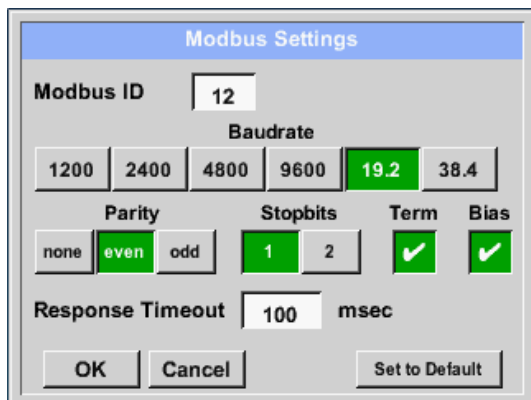

Please insert here the specified *Modbus ID* of the sensor, allowed values are 1 -247, (e.g. here *Modbus ID = 12*)

For setting the Modbus ID on the sensor, please see sensor-datasheet.

In addition in the menu are the serial transmission settings *Baudrate*, *Stopbits*, *Parity* and *Timeout* time to define.

In case that the DP 510 is the end of the RS485 bus system with activating *Term-* & *Bias-* button the required termination and biasing could be activated.

Confirmation by pressing *OK* button.

For resetting to the default values please press *Set to Default*.

## Sensor-Settings / Type „Modbus“

Main menu → Settings → Sensor settings → C1 → Reg. Address description field

The measurement values are kept in the registers of the sensor and can be addressed via Modbus and read by the DP 510.

This requires setting the desired register addresses in the DP 510

Entering the register / data address is here in decimal with 0-65535.

### Important:

Required is the correct register-address.

It should be noted that the register-number could be different to the register-address (Offset).

For this, please consult the sensor data sheet.

Main menu → Settings → Sensor settings → C1 → Reg. Format description field

With the buttons, *Input Register* and *Holding Register* the corresponding Modbus-register type will be selected.

The number format and transmission order of each value needs to be defined by *Data Type* and *Byte Order*. Both have to be applied in correct combination.

### Supported Data types:

|                   |                                  |    |                          |
|-------------------|----------------------------------|----|--------------------------|
| <b>Data Type:</b> | UI1 (8b) = unsigned Integer      | => | 0 - 255                  |
|                   | I1 (8b) = signed integer         | => | -128 - 127               |
|                   | UI2 (16b) = unsigned Integer     | => | 0 - 65535                |
|                   | I2 (16b) = signed integer        | => | -32768 - 32767           |
|                   | UI4 (32b) = unsigned Integer     | => | 0 - 4294967295           |
|                   | I4 (32b) = signed integer        | => | -2147483648 - 2147483647 |
|                   | R4 (32b) = floating point number |    |                          |

### Byte Order:

The size of each Modbus-register is 2 Byte. For a 32 bit value two Modbus register will be read out by the DS500. Accordingly for a 16bit Value only one register is read.

In the Modbus Specification, the sequence of the transmitted bytes is not defined clearly. To cover all possible cases, the byte sequence in the DS500 is adjustable and must adapted to the respective sensor. Please consult here for the sensor datasheet.


e.g.: High byte before Low Byte, High Word before Low Word etc.

Therefore, the settings have to be made in accordance to the sensor data sheet.

## Sensor-Settings / Type „Modbus“

### Example:


Holding Register - UI1(8b) - Value: 18

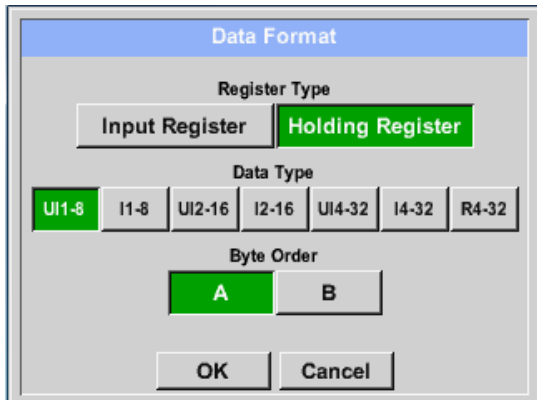

Selection Register Type *Holding Register*,  
Data Type *UI1(8b)* und Byte Order *A / B*

|            | HByte   | LByte   |
|------------|---------|---------|
| 18 =>      | 00      | 12      |
| Data Order | 1. Byte | 2. Byte |
| A          | 00      | 12      |
| B          | 12      | 00      |


Holding Register – UI4(32) - Value: 29235175522 → AE41 5652

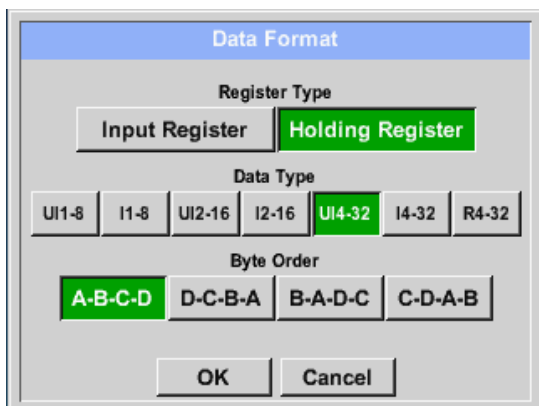

Selection Register Type *Holding Register*,  
Data Type *UI1(32b)* und Byte Order *A-B-C-D*

|                | HWord  |        | LWord  |        |
|----------------|--------|--------|--------|--------|
|                | HByte  | LByte  | HByte  | LByte  |
| 29235175522 => | AE     | 41     | 56     | 52     |
| Data Order     | 1.Byte | 2.Byte | 3.byte | 4.Byte |
| A-B-C-D        | AE     | 41     | 56     | 52     |
| D-C-B-A        | 52     | 56     | 41     | AE     |
| B-A-D-C        | 41     | AE     | 52     | 56     |
| C-D-A-B        | 56     | 52     | AE     | 41     |

Main menu → Settings → Sensor settings → C1 → Unit- description field

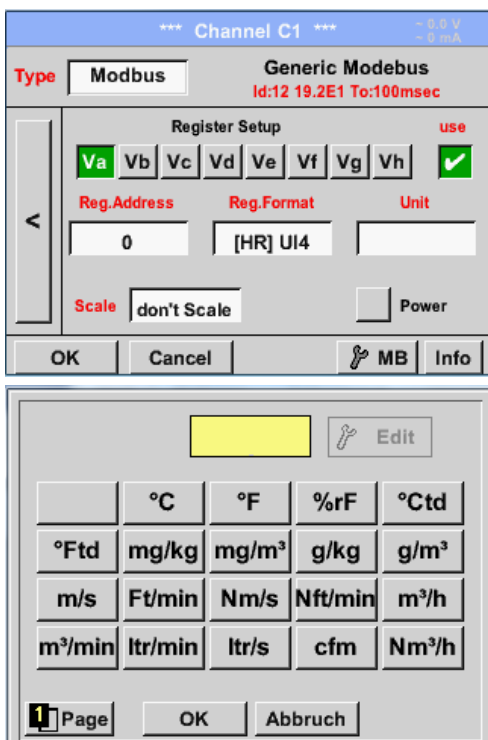

By pressing the description field *Unit*  
the list with the available units appear

Please select the unit by pressing the  
respective button e.g. *m³/h*.

For validation of the unit, please push the  
button *OK*

To move through the list please press the  
button *Page*.


In case the unit is **not** available, it is possible to  
create a user defined unit.

Therefore, please select one of the *User\_X*  
buttons.



## Sensor-Settings / Type „Modbus“


Main menu → Settings → Sensor settings → A1 → Scale- description field

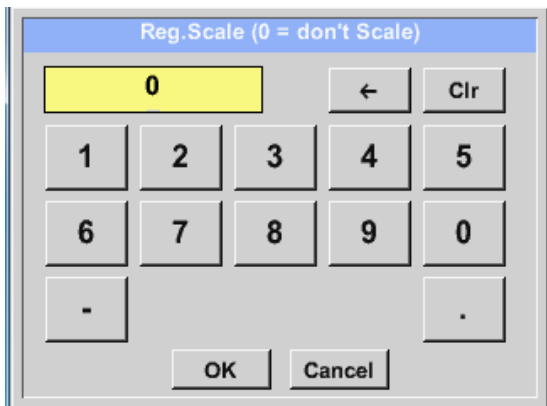

The use of this factor allows adapting the output value by the same.

By default or value = 0 no scaling is applied and displayed in the field is *don't scale*

Main menu → Settings → Sensor settings → C1 → OK

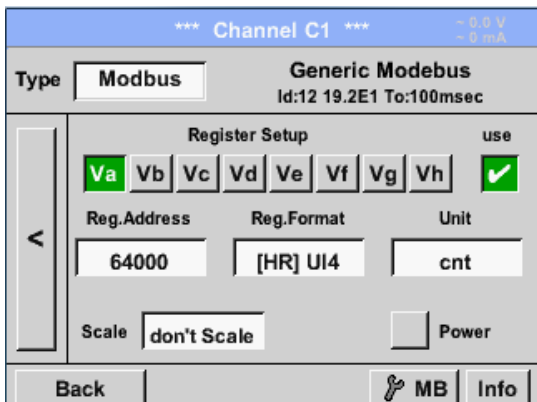


By pressing the *OK* button, the inputs are confirmed and stored.


## Data logger settings

### 10.3.2.5.5 Data logger Settings

Main menu → Settings → Logger settings

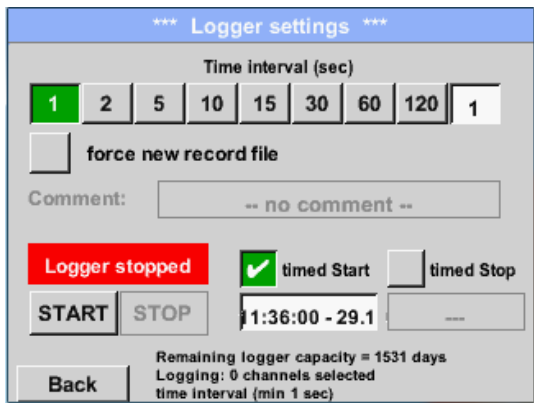

In the top row you can select the predefined *Time intervals* 1, 2, 5, 10, 15, 30, 60 and 120 seconds for recording.

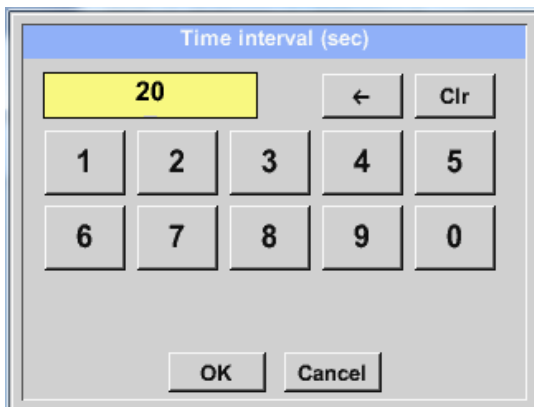

A different, individual *Time interval* can be entered in the highlighted white description field right at the head, where the currently set *Time interval* is always displayed.

**Remark:**

The largest possible *Time interval* is 300 seconds.

**Remark:**

If more than 12 measurement data are recorded at the same time, the smallest possible time interval of the data logger is 2 seconds.

And if more than 25 measurement data are recorded at the same time, the smallest possible time interval of the data logger is 5 seconds.

## Data logger settings

Main menu → Settings → Logger settings → force new Record File button

or

Main menu → Settings → Logger settings → force new Record File button → Comment description field

\*\*\* Logger settings \*\*\*

Time interval (sec)

1 2 5 10 15 30 60 120 1

force new record file

Comment: -- no comment --

Logger stopped  timed Start  timed Stop

START STOP 1:36:00 - 29.1

Back Remaining logger capacity = 1531 days  
Logging: 0 channels selected  
time interval (min 1 sec)

\*\*\* Logger settings \*\*\*

Time interval (sec)

1 2 5 10 15 30 60 120 1

force new record file

Comment: Messung 1

Logger stopped  timed Start  timed Stop

START STOP 1:36:00 - 29.1

Back Remaining logger capacity = 1531 days  
Logging: 0 channels selected  
time interval (min 1 sec)

A new recording file will be created by pushing the *force new record file* button and a name or comment can be entered by the choice of the *Comment* description field.

### Important:

If a new recording file should be created, the *force new record file* button must be activated. Otherwise, the last applied recording file is used.

Main menu → Settings → Logger settings → timed Start button

\*\*\* Logger settings \*\*\*

Time interval (sec)

1 2 5 10 15 30 60 120 1

force new record file

Comment: Messung 1

Logger stopped  timed Start  timed Stop

START STOP 1:36:00 - 29.1

Back Remaining logger capacity = 1531 days  
Logging: 0 channels selected  
time interval (min 1 sec)

By pushing the *timed Start* button and then the date/time description field below, the date and the start time can be set for a data logger recording.

### Remark:

If the start time is activated, it will automatically be set at the current time plus a minute.

## Data logger settings

Main menu → Settings → Logger settings → timed Stop button

\*\*\* Logger settings \*\*\*

Time interval (sec)

1 2 5 10 15 30 60 120 1

force new record file

Comment: Messung 1

Logger stopped

timed Start  timed Stop

START STOP 11:36:00 - 29.1 12:36:00 - 29.1

Back

Remaining logger capacity = 1531 days  
Logging: 0 channels selected  
time interval (min 1 sec)

By pushing the *timed Stop* button and then the date/time description field below, the date and the stop time can be set for a data logger recording.

**Remark:**

If the stop time activated, it will automatically be set to the current time plus an hour.

Main menu → Settings → Logger settings → timed Start button/timed Stop button  
→ Date/Time description field

timed Start

11 : 40 : 00 29 · 11 · 13 Cal

1 2 3 4 5


6 7 8 9 0

OK Cancel

After pushing the *date/time description field* a window will appear where the yellow marked area of the time or date can always be set and changed.


## Data logger settings

Main menu → Settings → Logger settings → timed Start button/timed Stop button  
→ Date/Time description field → Cal button

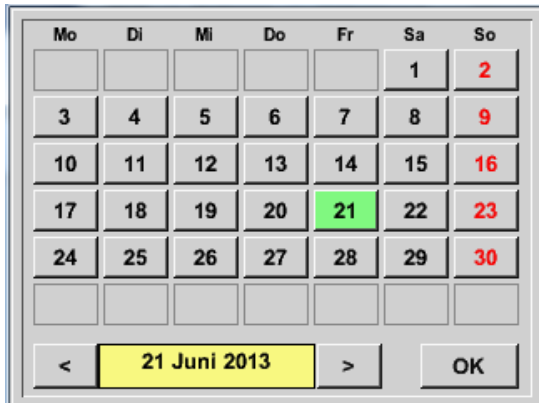

With the *Cal* button, the desired date can be easily select from the calendar.


Main menu → Settings → Logger settings → Start button

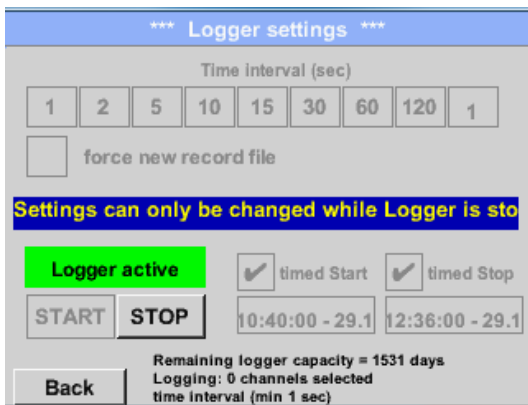

After the start and stop time activation and the created settings, the *Start* button will be pushed and the data logger is armed.

The data logger starts the recording at the set time!

Main menu → Settings → Logger settings → Start button/Stop button

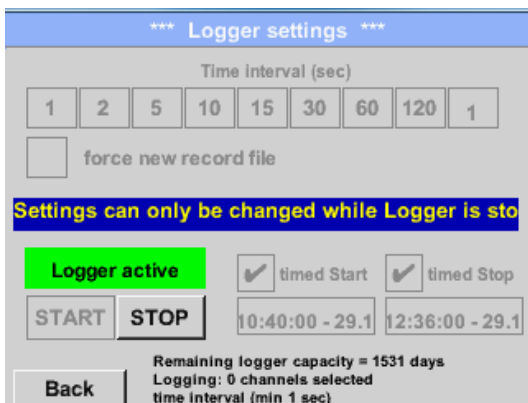

The data logger can be started without activated time settings, use the *Start* and *Stop* buttons for activate and disable. Left below there will be shown how many values are recorded and how long there still can be recorded.

**Remark:**  
The settings cannot be changed, if the data logger runs.

### Important:


If a new recording file should be created, the *force new record file* button must be activated. Otherwise, the last applied recording file is used.

## Device - Settings / Language

---

### 10.3.2.5.6 Device Settings


Main menu → Settings → Device settings

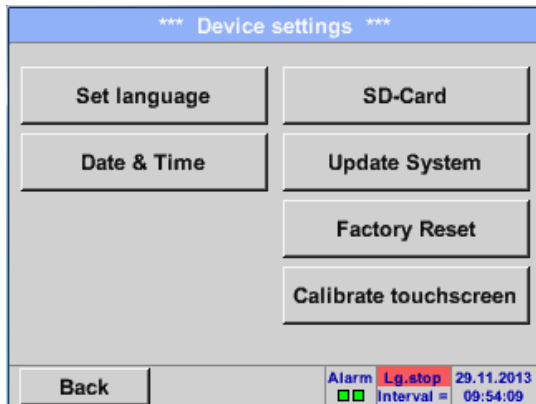

Overview of *Device settings*

### 10.3.2.5.6.1 Language

Main menu → Settings → Device settings → Set language

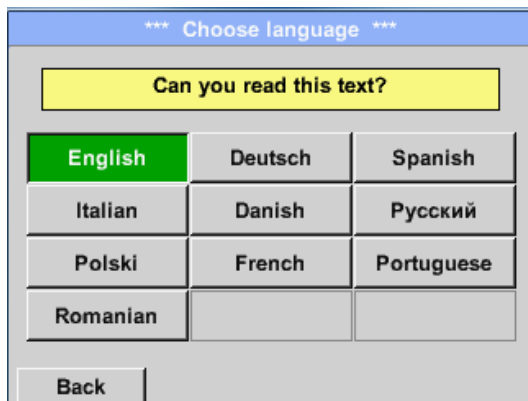

Here you can select one of 10 languages for the 500 / DP 510.

### 10.3.2.5.6.2 Date & Time

Main menu → Settings → Device settings → Date & Time

\*\*\* Time & Date Settings \*\*\*

Actual Time  Start

Time Zone UTC ±

Daylight Saving

Back Alarm Lg.stop 29.11.2013  
ty = 1531 09:55:18

By pushing the *Time Zone* description field and enter the correct *UTC*, you can set the correct time all over the world.

\*\*\* Time & Date Settings \*\*\*

Actual Time  Start

Time Zone UTC ±

Daylight Saving


Back Alarm Lg.stop 29.11.2013  
pacity = 1 10:55:43

The summer and wintertime switchover is realized by pushing the *Daylight Saving* button.

### 10.3.2.5.6.3 SD-Card

Main menu → Settings → Device settings → SD-Card → Reset Logger Database

Main menu → Settings → Device settings → SD-Card → Erase SdCard

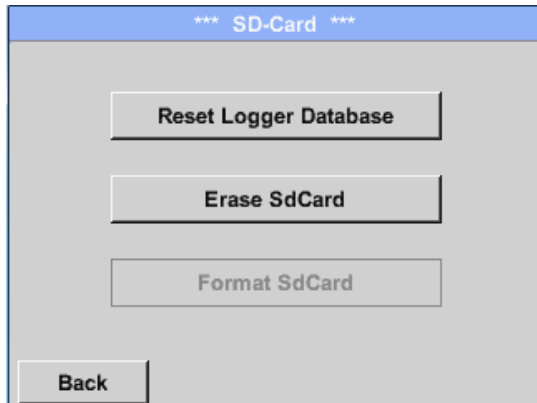

By pressing *Reset Logger Database* all actual stored data on SD-Card will be blocked for use in DS 400. Nevertheless all data are still stored and available for external use only.

By pressing *Erase SdCard* all Data on the SD-Card will be deleted.




## System / System Update

---

### 10.3.2.5.6.4 System update

#### Important!

System update can only be done with power supply connected to ensure there is a continuous power supply during the update.

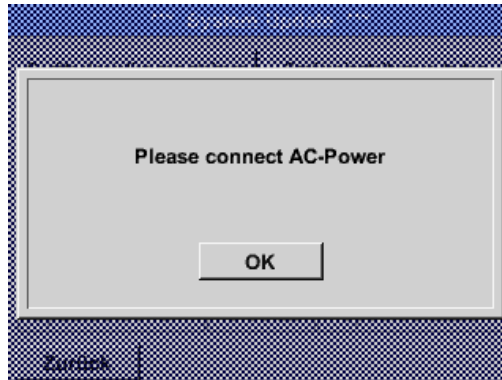


### 10.3.2.5.6.4.1 Save System Settings

#### Important:

Before updating the DP 500 / DP 510, the system settings should be secured either on a USB or on the internal SD-Card!

Home → Import / Export → Export System Settings

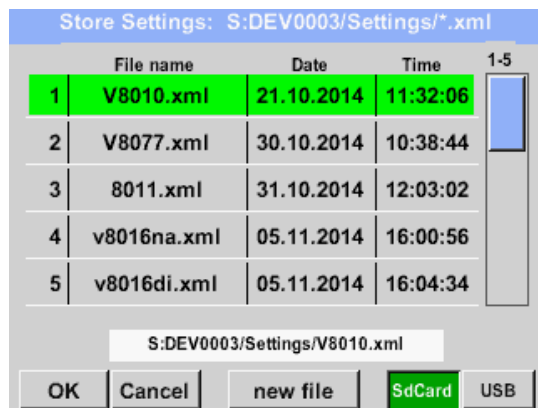

With Export system settings, all existing sensor settings can be exported to a USB stick or to the internal SD card. It stores all sensor settings including recording-, alarm-, graphics-, value- and name definitions. Storing location could be selected using the buttons *SD card* or *USB*.


Either a new file could be created by pressing "*new file*" or an existing file overwritten by selecting a name from the list.

The data are stored after confirmation with *OK*.


## System / System update

### 10.3.2.5.6.4.2 Check for new Software updates (USB)

Main menu → Settings → Device settings → Update System → Check USB Stick for new Software updates

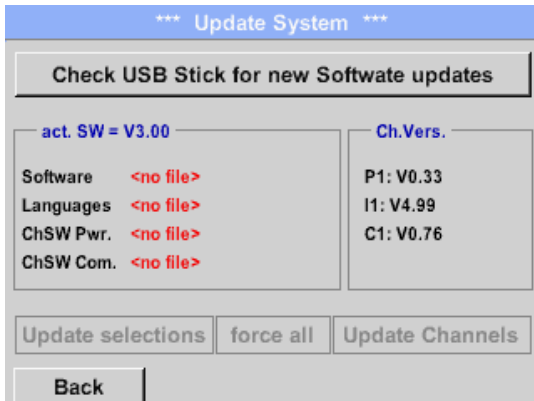

If after pushing the *Check USB Stick for new Software updates* button the following messages in the window appears, then DP 500 / DP 510 is not connected properly with the USB stick or no files are available.

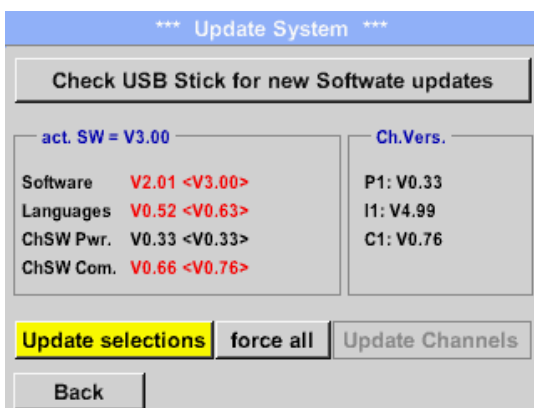

If the DP 500 / DP 510 is correctly connected to USB, and new version available it will displayed.

Right aside it shows the current (old) and another (new) available versions


Ist das DP 500 korrekt mit dem USB-Stick

Main menu → Settings → Device settings → System Update → Update selections

#### Important:

If the *Reboot system* button after the update appears, he must be pushed to restart the DP 500 / DP 510!

Main menu → Settings → Device settings → System Update → Update channels

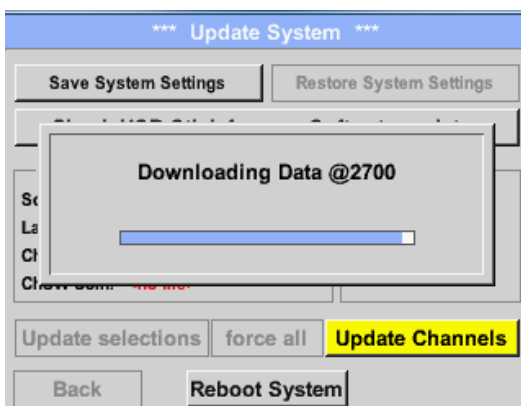

*Update* for the available *channels* of the DP 500 / DP 510.

#### Wichtig:

#### Important:


If after the channel update the *Reboot system* button appears, it has to be pushed to restart the DP 500 / DP 510.

Update of the channels maybe requires a repeating this procedures with a reboot of the system. In that case, after reboot of the system a popup is displayed.


# System / Factory Reset

## 10.3.2.5.6.5 Factory Reset

Main menu → Settings → Device settings → Factory Reset → Reset to Defaults

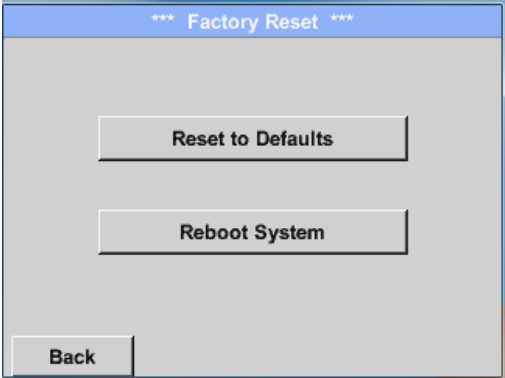



If necessary or required, by pressing the *Reboot System*-button the DP 500/510 DP could be rebooted.

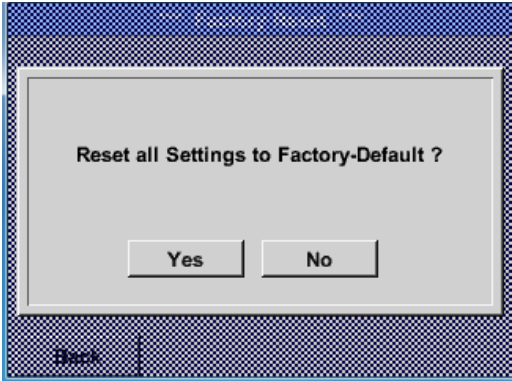

## Device - Settings / Cleaning and System Status

### 10.3.2.5.6.6 Calibrate touch-screen

Main menu → Settings → Device settings → calibrate touchscreen

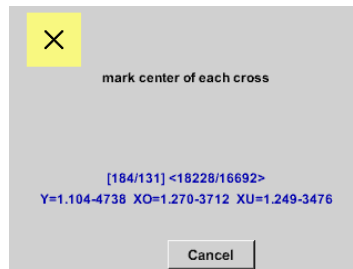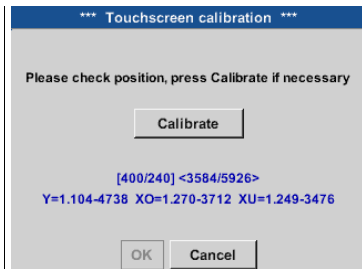

If necessary, the touch-screen calibration can be changed here. Push **Calibrate** and it appears, 1. left above, 2. bottom right, 3. bottom left, 4. right above and 5. in the middle, a calibration cross that must be pushed consecutively. If the calibration finished positive a message "**Calibration successful**" appears and have to be confirmed with **OK**. Is this not the case, so you can repeat the calibration with the help of the **Cancel** and **Calibrate** buttons.

### 10.3.2.5.7 Cleaning

Main menu → Settings → Cleaning




This function can be used for cleaning the touch panel during running measurements.

If one minute is not enough time to clean, the process can be repeated at any time.

Is the cleaning faster finished, then you can push the **to abort press long** button (for one or two seconds) to cancel.

### 10.3.2.5.8 System-Status

Main menu → Settings → System-Status

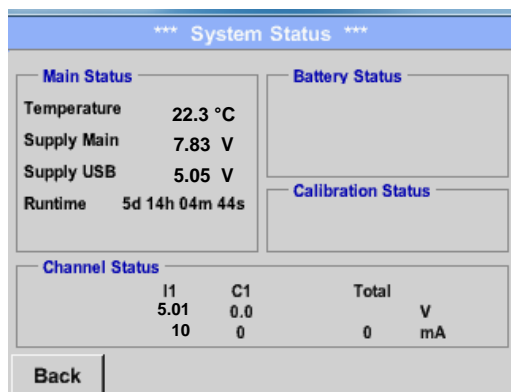

The function **System Status** offers an overview, fitting voltages and currents on the individual and the entire channel, as well as the power supply of the power supply unit.

By the **Runtime**, you always know how long the DP 500 / DP 510 was in total in operation

## System / System update

---

### 10.3.2.5.9 About DP 500 / DP 510

Main menu → Settings → About DP 510



Brief description of the **Hardware** and **Software Version**, as well as the **Serial Number** of the DP 500 /DP 510.

Under options, you can buy two additional, different functions (only DP 510 , if you have not done this by ordering).

# Chart

## 10.3.2.6 Chart


Main menu → Chart

**Attention:**

In the **Chart**, there can be represented only records that have already finished!

Current records can be seen in *Chart/Real time values*.

(See chapter 10.3.2.3 Chart/real time values)

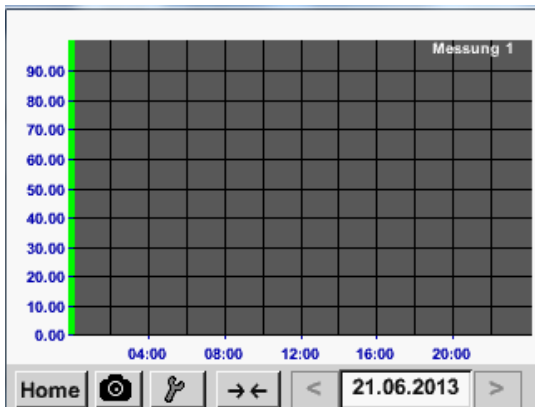


Running measurement, there are no values represented!

Zoom and scroll options in the time domain of the *Chart*:

→ ← Maximal an entire day can be represented (24h).

← → The smallest possible range is represented, depending on the time interval of the recording.

Additional zooming and scrolling options in *Chart* and *Chart/Real time values*

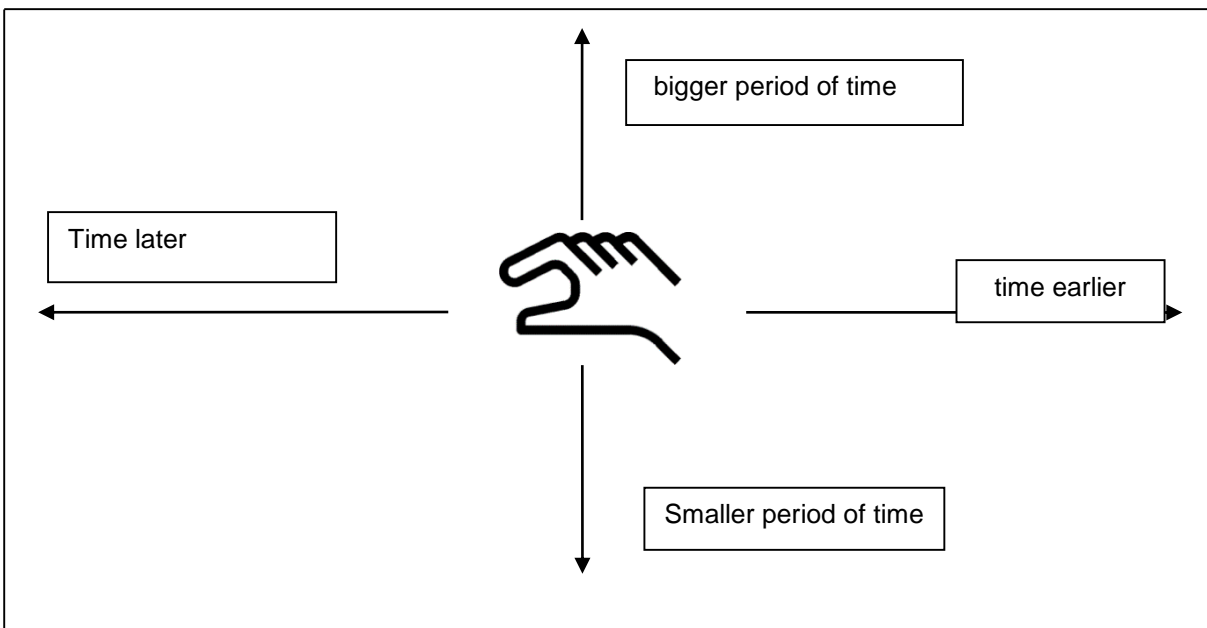


# Chart

Main menu → Chart → Date description field




By pushing the **date** description field (center bottom) the calendar, from which the appropriate date can be selected conveniently, appears.

Stored measuring data can be select here by **time** (**START** and **STOP**), **Comment** and **File name** (contains English date).

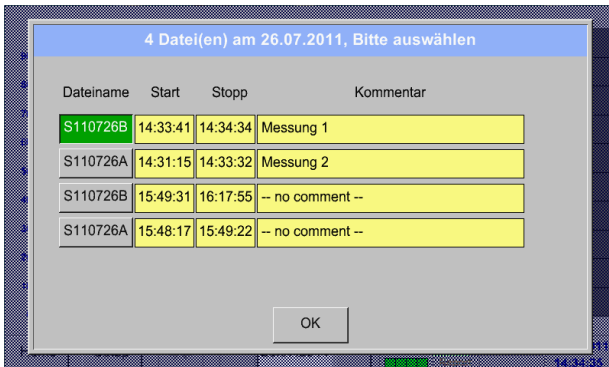

Main menu → Chart → Setup

In the **Setup**, you can make up to four different y-axis labels and in addition choose a **Unit**, the grid (**min**, **max**, **step**) and several channels (**Plots**) and a **Colour**.

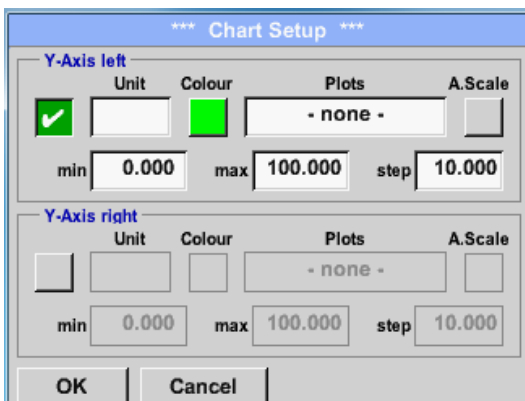

The y-axis **left** is already enabled, you can choose a **Colour** for it.

**Remark:**  
Grid setting is already possible at this point, but later when a record is selected, it is more reasonable!

# Chart


Main menu → Chart → Setup → Unit description field



Select the *Unit* of the represented recording from the menu.




Main menu → Chart →

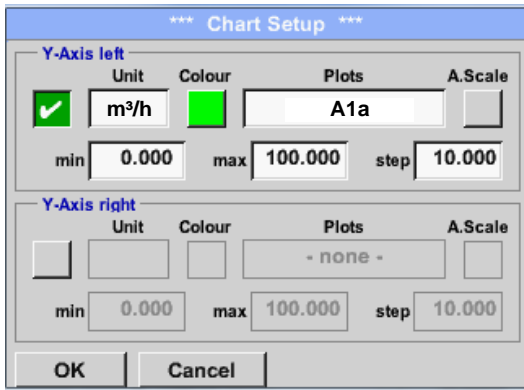

Now, the grid can be set with *min*, *max*, and *step*.

By pushing the *A.Scale*-button a calculated auto-scaling will be defined.

In the same way the remaining y-axes can be labelled!

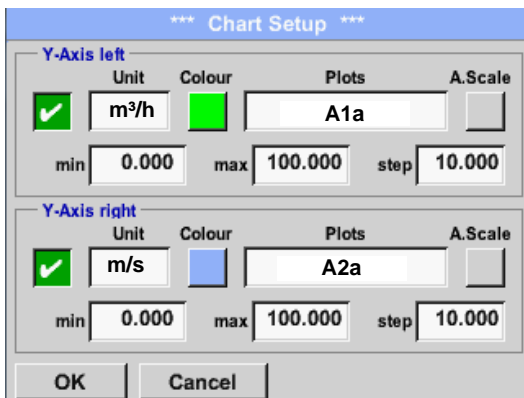


Two different grid settings with various *Units* and *Colours*.



# Chart


Main menu → Chart

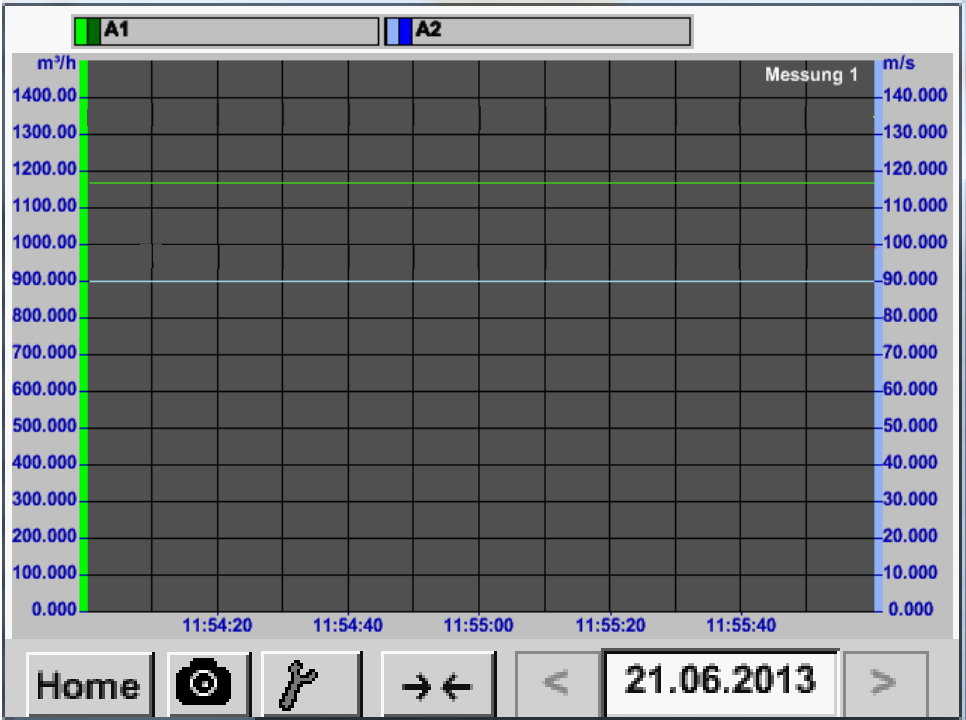

# Chart / Real time values

## 10.3.2.7 Chart / Real time values

Main menu → Chart/Real time values

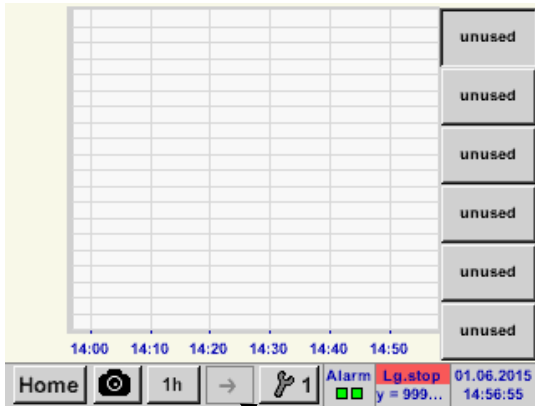


One or more channels for the recording and presentation of measured data can be selected here, such as a dew point sensor or several different sensors.


After pushing this button currently recorded measurement data in the current time range are represented.

Quick access to predefined time periods 24 h, 8 h, 1 h, 15 min and 2 min. At the push of a button the chart for the selected time range is displayed.

Main menu → Chart/Real time values →  #1- #6

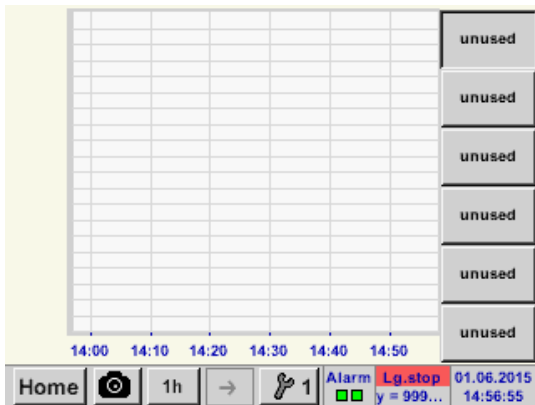

In this menu item, up to twelve channels (depending on the version of the DS 400) can be activated at the same time and viewed in *Main → Chart/Real time values*.

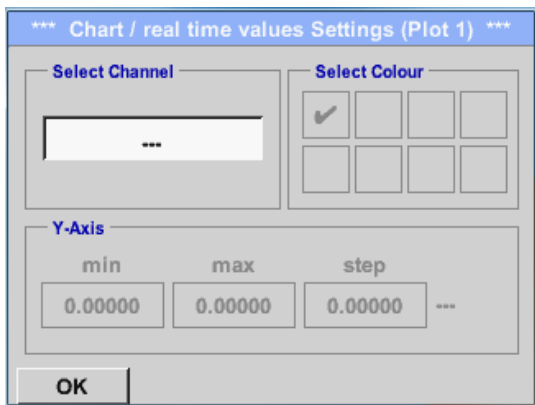


Here the channel C1 chosen.

For each channel, you can select a value to be represented in the *Chart* and one to display (*2. values*).

In addition, it can be set, like in *Main → Chart*, a *colour* and the grid (*min, max, step*) of the y-axis.

## Chart / Real time values

Main menu → Chart/ Real time values

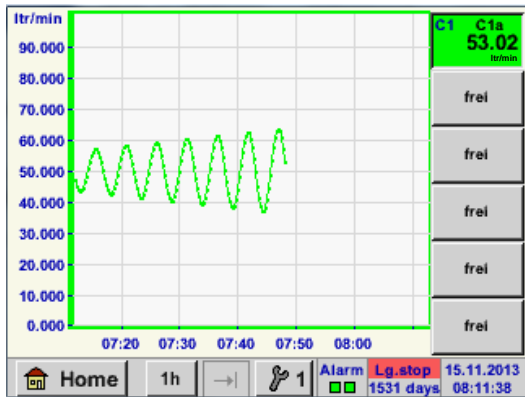

### Channel C1:

Elected the flow as *Chart*

If several channels are logged, all charts will be displayed, but there is only the y-axis of the selected channel visible.


If there is no grid entered in the setup, *min* will be 0, *max* 100 and *step* 10

In the same way, the remaining setups can be set!

# Channels

## 10.3.2.8 Channels


Main menu → Channels

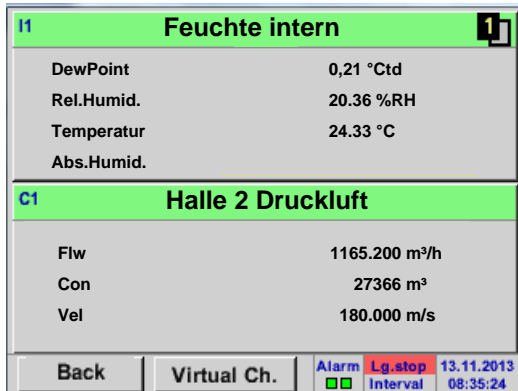

The overview of *Channels* shows the current measured values of all connected sensors.

Exceeds or falls below the set alarm limits, the respective measured value flashes yellow (*alarm 1*) or red (*alarm 2*).

Main menu → Channels → C1

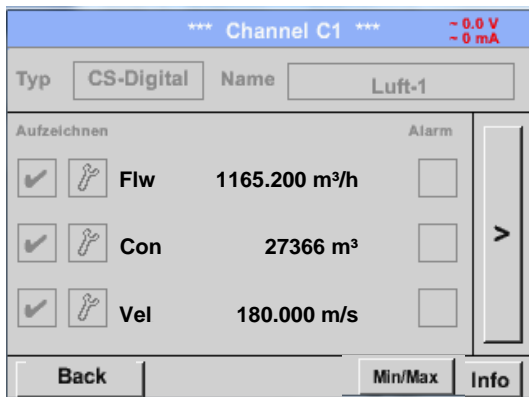


Each channel can be selected and the settings viewed and checked, but **no changes** can be made here.

**Remark:**  
Please, make changes in the *Settings!*

### 10.3.2.8.1 Min/Max Function

This feature allows reading out the minimum or maximum values of the current measurement for each connected sensor. Start of recording is immediately after setting of the sensor, but there is always the possibility to reset the Min and Max values.

Main menu → Channels → I1 → **Min/Max**

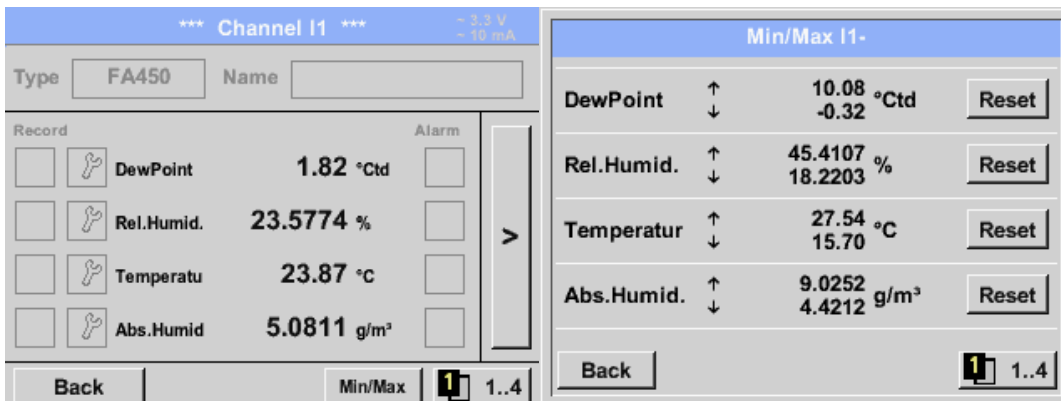


↑ = Max-Wert ↓ = Min-Wert

## Channels

---

Main menu → Channels → I1 → **Min/Max** → Dew point **Reset**

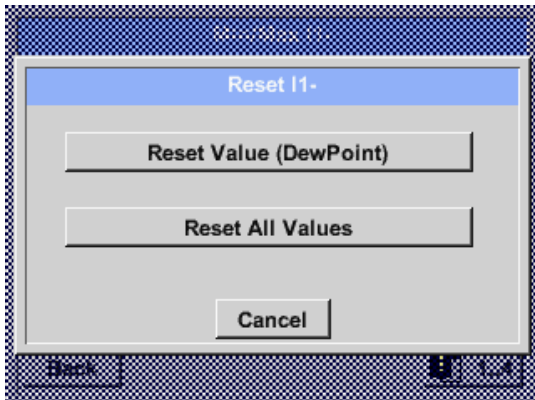


It is possible to reset a single measurement value, here it is the dew point or if needed to reset all minimum and maximum values of the sensor.

**For resetting the single value the *Reset Value* –Button for all Min/Max-Values the *Reset All Values* –Button has to be pressed.**

# Real time values

## 10.3.2.9 Real time values

Main menu → Real time values

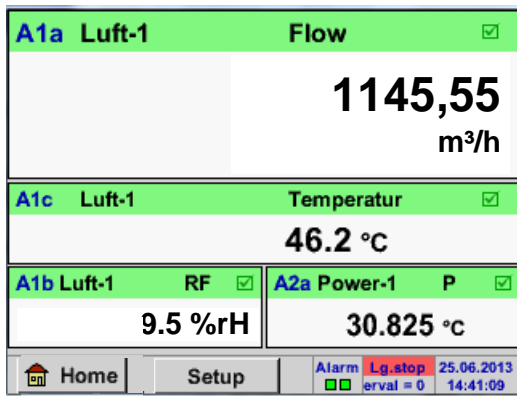


The view *Real time values* allows displaying of 1 to 5 free definable measurement values.

By exceeding the upper- or lower alarm levels the respective measurement value flashes yellow for *Alarm-1* or red for *Alarm-2*.

**Remark:**  
Changes for display settings have to be done in the *Setup* menu!

Main menu → Real time values → Setup → next Layout

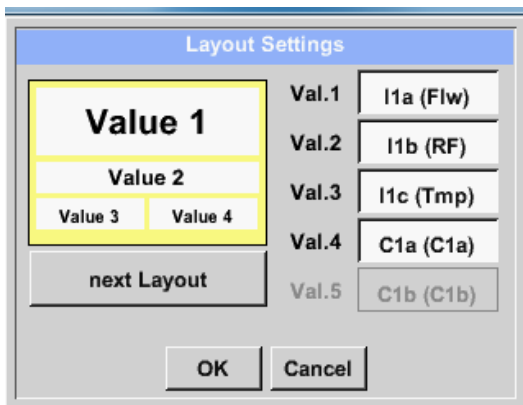


Here, by pressing *next Layout*-button it is possible to select the wanted layout.

You can choose between 6 different layouts showing 1-5 measurements. see below.

The values to be displayed could be selected in the *Val.1 to Val.5* description fields.


Different variants:

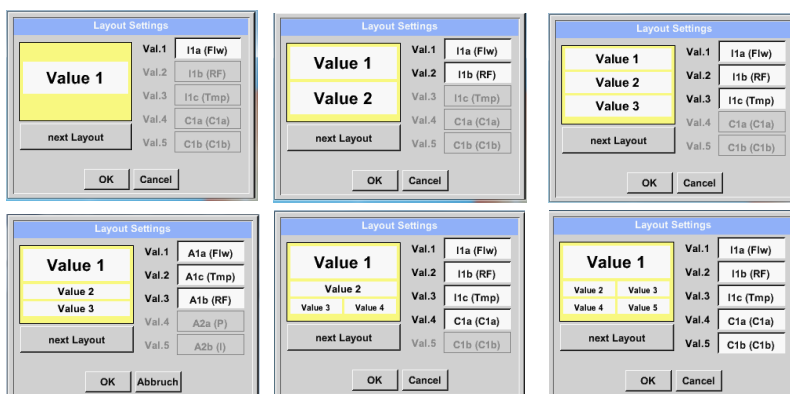

# Alarm overview

## 10.3.2.10 Alarm overview


Main menu → Alarm-Overview

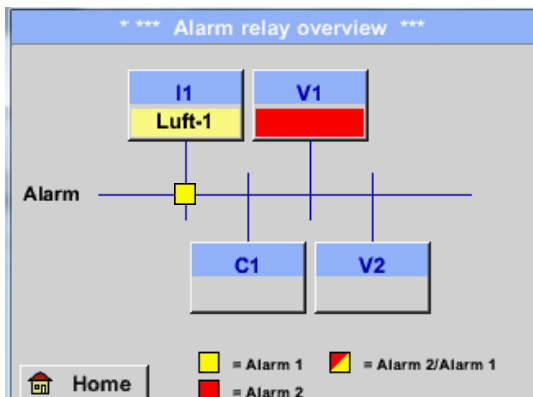

In the Alarm overview, you can immediately see whether there is an *alarm 1* or *alarm 2*. You can see also in other menu items:  
*Main* → *Real time values* and  
*Main* → *Settings* → *Sensor settings*  
The channel name will appear yellow inverts (*alarm 1*) or inverse red (*alarm 2*).  
In addition, you can see which popup had been set for the channel as the *alarm 1* or *alarm 2*.

Here *Alarm-1* for Channel I1!

Main menu → Alarm-Overview → C1

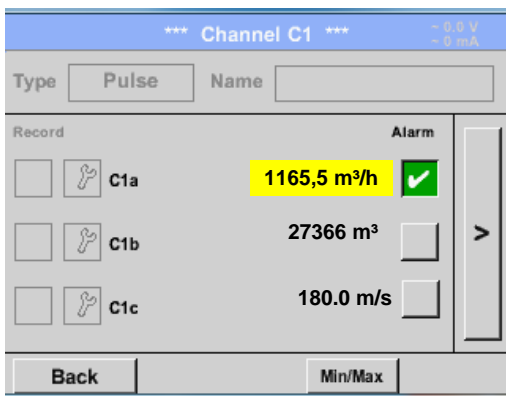

Like in *Main* → *Real time values*, individual channels can be selected here, to detect which and how much the value has exceeded or below the alarm range.

**Remark:**  
The alarm parameters can be set and/or modified here.

### 11 Virtual Channels (optional)

The option „Virtual Channels“ offers 4 additional channels (no HW Channels) where it is possible to display calculations of each single HW-Channel, virtual channels and free defined constants as well. For each „Virtual Channel“ are 8 calculations each with of 3 operands and 2 operations possible.


Possible cases are calculation of:

- Specific performance of a compressor(s)
- Complete consumption of a compressor( or the sum of several compressors)
- Energy cost etc.

#### 11.1 Option „Virtual Channels“ activation

After purchasing of the option „Virtual Channels“ the functionality have to be activated first.

Main menu → Settings → About DP 510

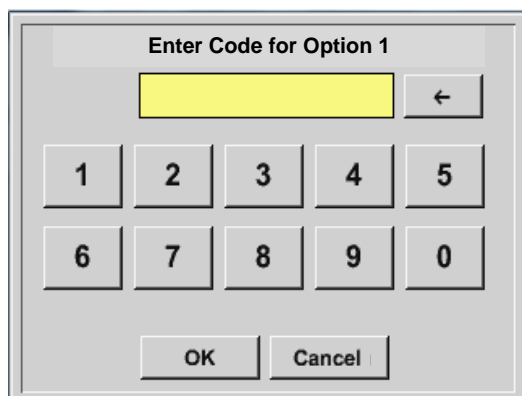

Please push the button Buy for „Virtual Channels“ and you will requested to insert the key-code received


Please enter the Key-Code in the text-field and activate the option by pushing the button **OK**



# Virtual Channels

## 11.2 Virtual Channels Settings

Main menu → Settings → Sensor Settings → Virtual Channels

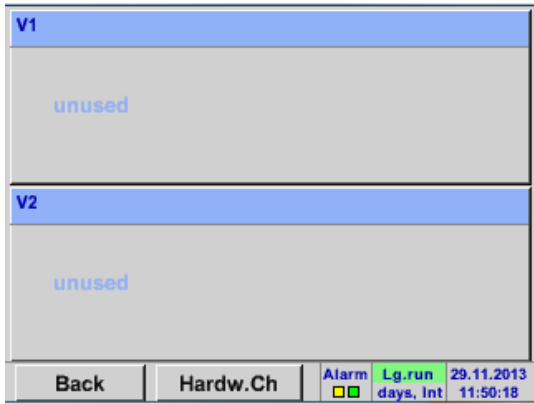


After pushing the button „*Virtual Channels*“ in the Sensor Settings menu an overview with the 4 available “*Virtual Channels*” is displayed.

**Remark:**  
By default all channels are without settings.


### 11.2.1 Selection of Sensor-type

Main menu → Settings → Sensor Settings → Virtual Channels → V1

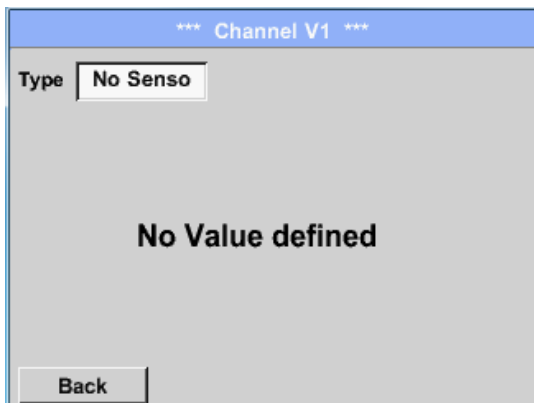

By pushing the description field *Type No Sensor* the list of sensor types appears (see next step).

Main menu → Settings → Sensor Settings → Virtual Channels → V1 → Type description field

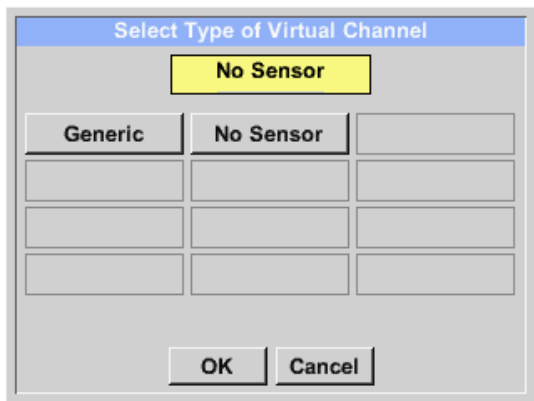

If still no sensor has been configured, the *Type No Sensor* appears.

By pushing the button **Generic** the virtual channel is selected.  
Pushing the button **No Sensor** will reset the virtual channel.

Confirmation of selection is done by pressing the button **OK**.

## Virtual Channels

Main menu → Settings → Sensor Settings → Virtual Channels → V1 → Name description field

By pushing the Text field *Name* a Sensor name could be inserted.

### 11.2.2 Configuration of each single virtual value

Each virtual channel includes 8 individual calculated values where every value has to be activated separately.

### 11.2.3 Activation of a single virtual value

Main menu → Settings → Sensor Settings → Virtual Channels → V1 → arrow right (2.page) → V1a → Use

Every virtual value has to be activated by selecting the respective *Value-Button* e.g. *V1a* and pushing of the *Use Button*.


### 11.2.4 Definition of Operands

Main menu → Settings → Sensor Settings → Virtual Channels → V1 → arrow right (2.page) → 1stOperand


By accessing the text field *1st Operand* The list with all channels (HW and virtual channels) and const. Value appears.

## Virtual Channels


Main menu → Settings → Sensor Settings → Virtual Channels → V1 → arrow right (2.page) → 1stOperand → C1

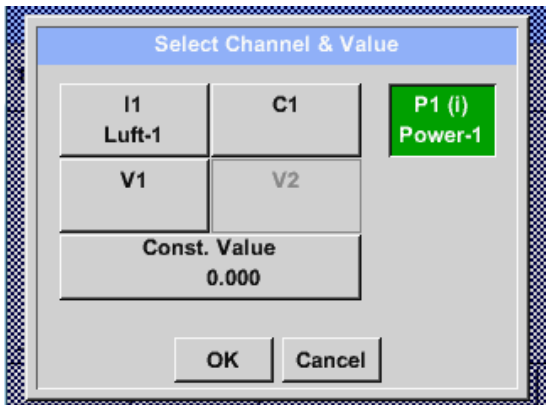

By pressing a button either for HW-, virtual channel or const. Value e.g. **C1** a list of all available measurement channels or measurement values will appear.

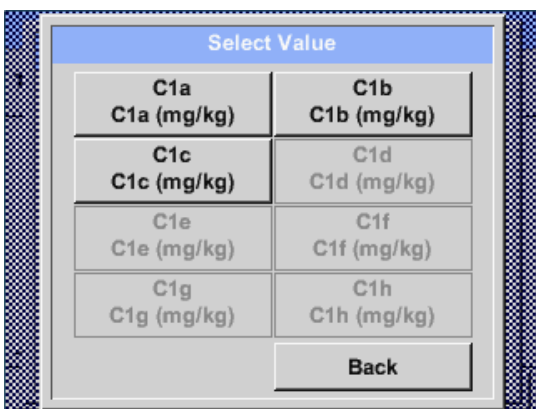

Pressing the respective channel button e.g. **C1b** will select the measurement channel

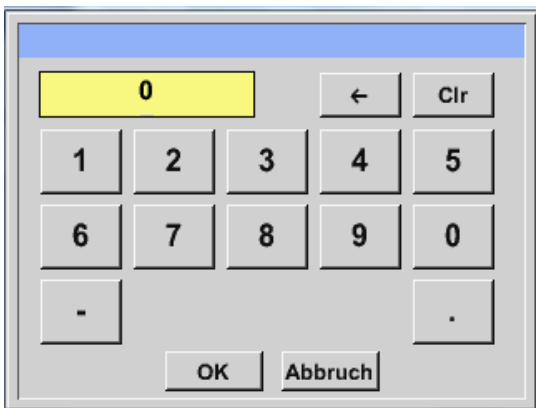

Pressing the button **const. Value** requests the input of the **const. Value** into the text field.

With button **OK** the value will validated

With the buttons **←** and **Clr** it is possible to correct the input.

Button **←** deletes the last figure

Button **Clr** clears the whole field

This approach is analogous to the other operands. (1st Operand, 2nd Operand and 3rd Operand).

## Virtual Channels

### 11.2.5 Definition of Operations

Main menu → Settings → Sensor Settings → Virtual Channels → V1 → arrow right (2.page) → 1st Operation



By accessing the text field *1st Operation* the list with all available operands appears.


Selecting and validation of the operand by pressing the respective operand.

Pressing of the button *not used* deactivates the operation of the dedicated operand.


This approach is analogous for both operations (1st Operation and 2nd Operation)

### 11.2.6 Definition of Unit

Main menu → Settings → Sensor Settings → Virtual Channels → V1 → arrow right (2.page) → Unit

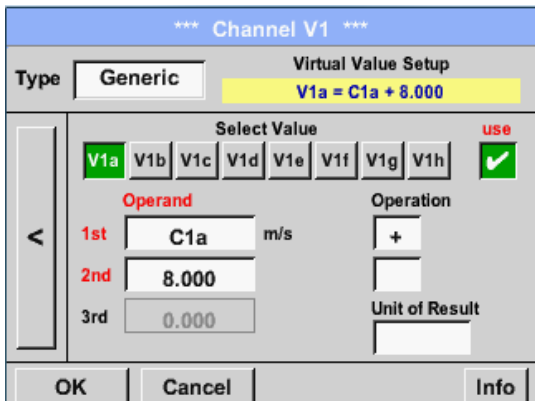


By accessing the text field *Unit of Result* the list with all available units appears

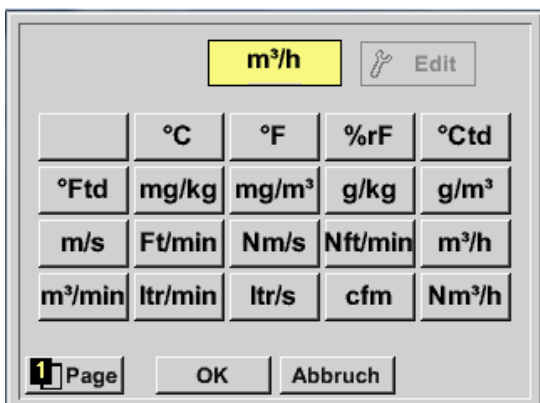


Please select the unit by pressing the respective button e.g. *m³/h*.  
For validation of the unit please push the button *OK*.  
To move through the list please press the button *Page*.  
In case the unit is **not** available it is possible to create a user defined unit.  
Therefore, please select one of the *User\_X* buttons.

## Virtual Channels

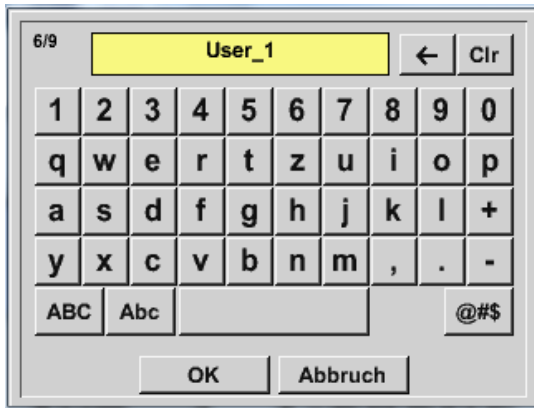

By pressing the button *Edit* you enter the menu for inserting the new Unit.

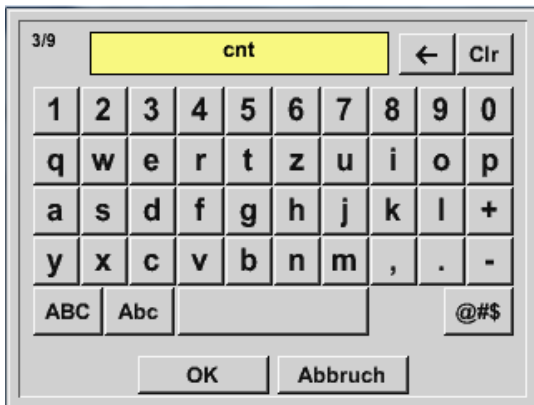

Then define the unit and confirm it with the button *OK*.

With the buttons *←* and *Clr* it is possible to correct the input.

Button *←* deletes the last figure  
Button *Clr* clears the whole field

### **Important**

Each calculation allows you the use of maximum 3 operands and 2 operations.


The calculation is then based on following formula:

**Example:**     **V1a = (1st Operand 1st operation 2nd Operand) 2nd operation 3rd Operand**  
                  **V1a = (A1c – A2a) \* 4.6**


## Virtual Channels

### 11.2.7 Value name, resolution of decimal places and recording of values

Main menu → Settings → Sensor Settings → Virtual Channels → V1 → Tool-Button

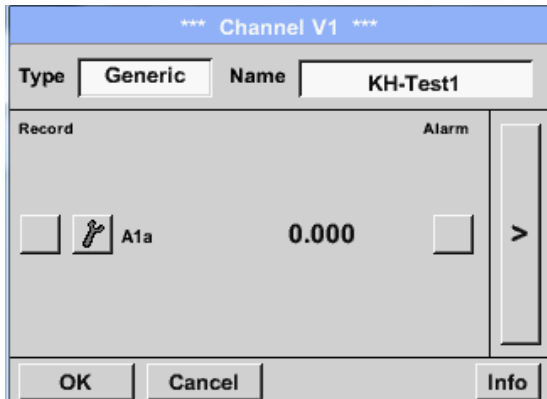

The *Resolution* of the decimal places, the *Short Name* and *Value Name* are found under the **Tool button**

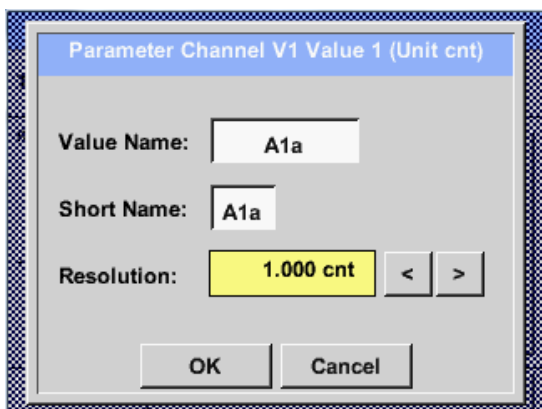


For the recorded *Value* there can be entered a *Name* with 10 characters and later in menu item *Graphics/Real time values* it is easier to identify it.

Default names are e.g. *V1a*.  
*V1* is the Channel name, *a* is the first measuring value of channel V1, *b* is the second measuring value and *c* the third etc.

The *Resolution* of the decimal places is simply adjustable by pushing right and left

Main menu → Settings → Sensor Settings → Virtual Channels → V1 → Record Button

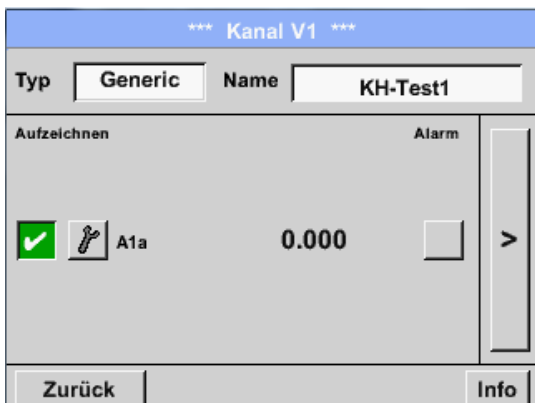

Use the *Record* buttons to select the measurement data that will be stored by **activated data logger**

#### **Attention:**

Before the selected measurement data are recorded, the data logger must be activated after the settings (See chapter [10.2 Logger-Settings \(Data logger\)](#)).

See also chapter [10.3.2.1.2.3 Name the measurement](#) and [10.3.2.1.2.4 Recording measurement data](#)

### 12 Analog Total (optional only for DP 510)

The Option „Analog Total“ offers the possibility of a consumption measurement also for sensors with analogue outputs e.g.: 0-1/10/30V and 0/4 – 20mA.


#### 12.1 Option „Analog Total“ activation

After purchasing of the option „Analog Total“ the functionality has to be activated first.

Main menu → Settings → about DP 510



Please push the button *Buy* for „Analog Total“ and you will be requested to insert the key-code received

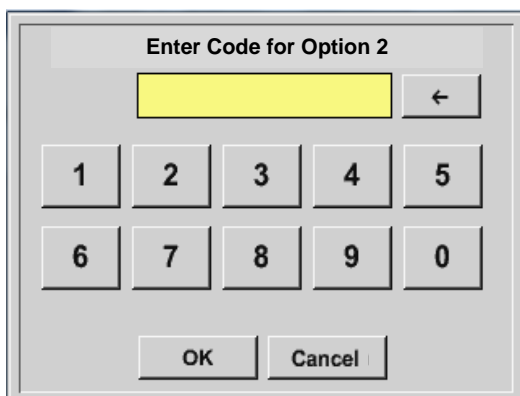


Please enter the Key-Code in the text-field and activate the option by pushing the button *OK*.

# Analog Total

## 12.2 Selection of sensor type

See also Chapter [10.3.2.1.2.9 Configuration of analogue sensors](#)


Main menu → Settings → Sensor Settings → C1

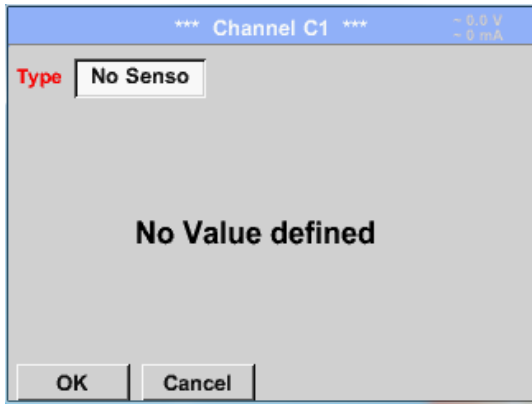

If still no sensor has been configured, the **Type No Sensor** appears.


By pushing the description field **Type No Sensor** the list of sensor types appears (see next step).

Main menu → Settings → Sensor Settings → C1 → Type description field

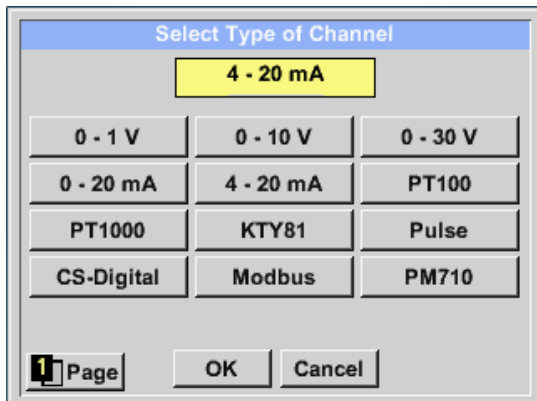

By pushing the button of the required sensor button e.g. 4 -20mA the sensor is selected. Pushing the button **No Sensor** will reset the selection.

Confirmation of selection is done by pressing the button **OK**.

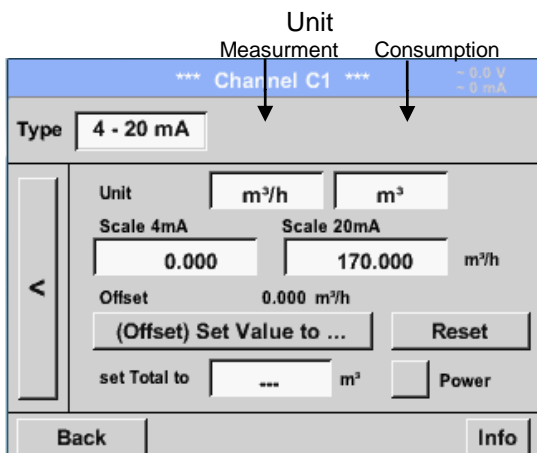

Selection of the units by pushing the text fields for the corresponding measurement and consumption units.

In addition, you can push the **scale buttons** for the min. and max. scaling values and set the measuring range.

Here we have **0 m³/h** for 4 mA and **170m³/h** for 20mA

In addition it is possible to enter a starting value for consumption entering **set Total to** field e.g. to take over value from an old counter.

### Remark:

The text field „Unit-Consumption“ is only editable in case of measurement values (Units) with volume per time unit and thus also the consumption calculation.


For labelling and setting of the description fields see also chapter [10.3.2.1.2.8 label and setting the description field](#)



## 13 Export /Import

Recorded data can be transferred to a USB stick, by using *Export/ Import*.

Main menu → Export / Import

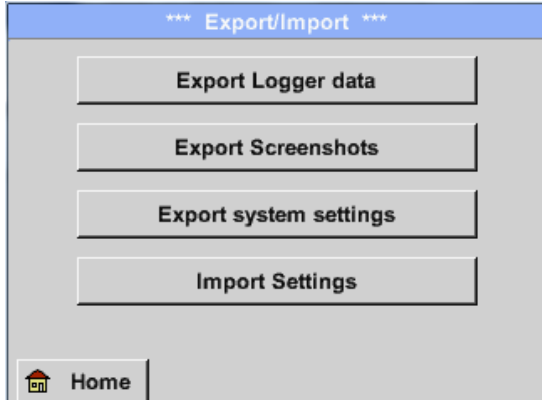


With *Export Logger data*, *Export Screenshots* and *Export system settings* the recorded measurement data, screenshots and saved settings can be transferred to a USB stick.

With *Import Settings* saved system settings could be imported from USB stick or SD card.


### 13.1 Export Logger data

Main menu → Export data → Export Logger data

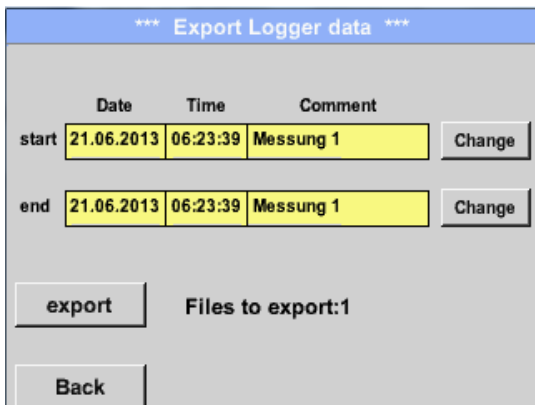

Use the *Change* buttons to adjust a period between *start* and *end*. Stored measurement data in this period are exported.

Main menu → Export data → Export Logger data → Change

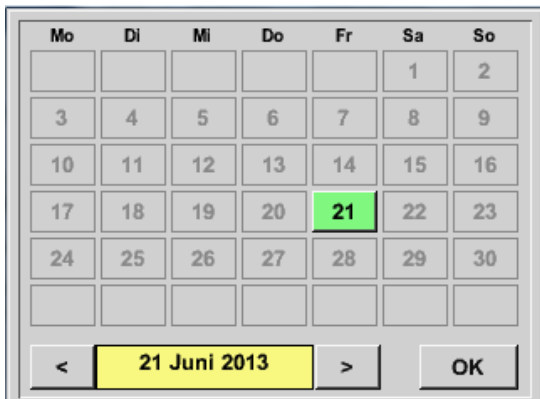


The selected date is always green, and the date numbers of the Sundays are red, like in the calendar.

On days, where measurement data were recorded, the date numbers are optical highlighted.

## Analog Total

---

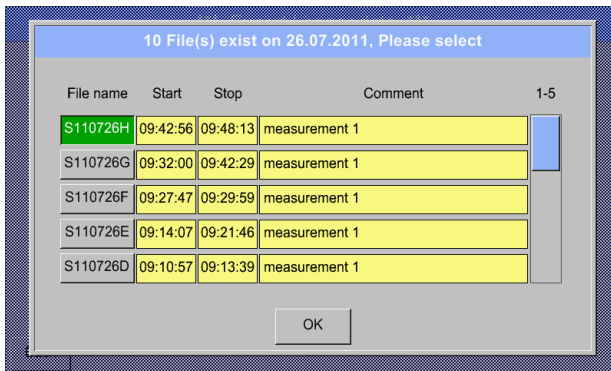

If there have been recorded several measurements on the same date, they appear after the date selection with **OK**.

Now a recording can be selected comfortable.


Main menu → Export data → Export Logger data → export

The measurement data of the selected period are exported to a USB stick.

### 13.2 Export System Settings

Using this function, all existing device- and sensor settings can be exported to a USB stick or SD-card. All sensor settings including recording-, alarm-, measurement resolution-, graphics-, current values- and naming-definitions are taken over.

Main menu → Export/Import → Export system settings

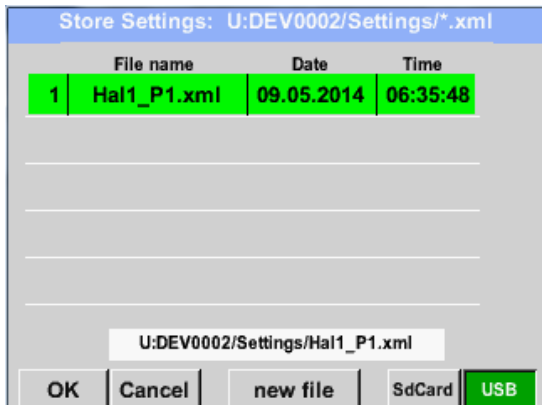

All already saved system settings will be displayed, depending on the location USB Stick or SD-Card..

Location/ path is : DEV0003/Settings

In case an existing file will be selected, the content will be overwritten with the new settings after confirming with **OK**.

New File storage:

Select the location for storing by pressing the button **USB** or **SdCard**.

By choosing button **new file** a menu for inserting/defining the filename appears.

The file name length is limited **to 8 chars**.


File save/confirm with: **OK → OK**

### 13.3 Import System Settings

Using this function, stored system settings can be read back again.

All sensor settings including recording-, alarm-, measurement resolution-, graphics-, current values- and naming-definitions are taken over.

Main menu → Export/Import → Import system settings

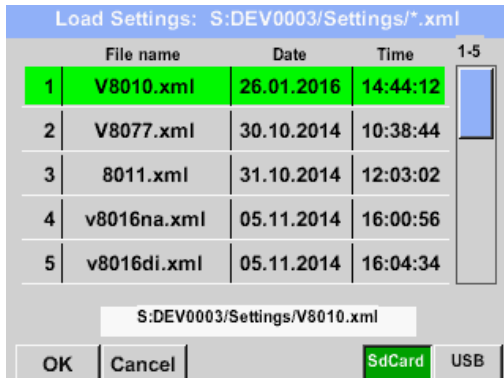

Depending on the selected location, USB stick or internal SD-card, all already stored settings will be listed.

Selection of storage location by pressing button **USB** or **SdCard**

The selected file be imported after confirming with **OK**.

To avoid any unwanted overriding of the actual device settings it is an additional confirmation required

After importing of the new settings a reboot is required too.

For the complete takeover of the new sensor settings, they have to be activated for each channel too.

Main menu → Settings → Sensor Settings → Channel A1 ...B2

Stand: 22/03/2016, V1.30

# KONFORMITÄTSERKLÄRUNG

DECLARATION OF CONFORMITY

Wir CS Instruments GmbH  
We Am Oser 28c, 24955 Harrislee

Erklären in alleiniger Verantwortung, dass das Produkt  
Declare under our sole responsibility that the product

**Mobile Taupunkt –Messgeräte DP 500 / DP 510**  
Portable dew point meters DP 500 / DP 510

den Anforderungen folgender Richtlinien entsprechen:  
We hereby declare that above mentioned components comply with requirements of the following EU directives:

|   |                          |
|---|--------------------------|
| Elektromagnetische Verträglichkeit<br>Electromagnetic compatibility | 2014/30/EU<br>2014/30/EC |
|---|--------------------------|

Angewandte harmonisierte Normen:

Harmonised standards applied:

|                                       |  |
|---------------------------------------|--|
| EMV-Anforderungen<br>EMC requirements | <b>EN 61326-1: 2006-10 2013-07</b><br><b>EN 61000-3-2 : 2015-3</b> |
|---------------------------------------|--|

Anbringungsjahr der CE Kennzeichnung: 13

Year of first marking with CE Label: 13

Das Produkt ist mit dem abgebildeten Zeichen gekennzeichnet.  
The product is labled with the indicated mark.



Harrislee, den 19.04.2016

  
Wolfgang Blessing Geschäftsführer



报告编号(Report ID): H11133012221D~1

# 锂电池UN38.3测试报告

## Lithium Battery UN38.3 Test Report

|                              |                             |
|------------------------------|-----------------------------|
| 样品名称<br>(Sample Description) | Lithium-ion Battery 238700  |
| 委托单位<br>(Applicant)          | Jauch Quartz GmbH-Batteries |
| 生产单位<br>(Manufacturer)       | Jauch Quartz GmbH-Batteries |



No.: H11133012221D  
Code: ssak93kqv



Pony Testing International Group

I. SAMPLE DESCRIPTION

|                      |                             |                                   |               |                        |             |
|----------------------|-----------------------------|-----------------------------------|---------------|------------------------|-------------|
| Sample Name          | Lithium-ion Battery         |                                   | Battery Type  | 238700                 |             |
| Client               | Jauch Quartz GmbH-Batteries |                                   |               |                        |             |
| Manufacturer         | Jauch Quartz GmbH-Batteries |                                   |               |                        |             |
| Nominal Voltage      | 7.2V                        | Rated Capacity                    | 2600mAh       | Limited Charge Voltage | 8.56±0.025V |
| Charge Current       | 1250mA                      | Maximum Continuous Charge Current | 2600mA        | End Charge Current     | 100mA       |
| Cut-off Voltage      | 5.5V                        | Maximum Discharge Current         | 5200mA        | Use                    | ---         |
| Cells Number         | 2PCS                        | Cell Model                        | 18650         | Rated Capacity         | 2600mAh     |
| Manufacturer of cell | Samsung SDI Co., Ltd        |                                   |               |                        |             |
| Chemical component   | Li-Ion                      |                                   |               |                        |             |
| Client date          | 2013-11-12                  |                                   | Finished date | 2013-12-02             |             |

II. REFERENCE METHOD

《United Nations Recommendations On The Transport Of Dangerous Goods, Manual Of Tests And Criteria》(ST/SG/AC.10/11/Rev.5/Amend.1).

III. TEST ITEM

- |                        |                           |
|------------------------|---------------------------|
| 1. Altitude simulation | 5. External short circuit |
| 2. Thermal test        | 6. Impact                 |
| 3. Vibration           | 7. Overcharge             |
| 4. Shock               | 8. Forced discharge       |

IV. CONCLUSION

| ITEM                   | SAMPLE NUMBER  | STANDARD | CONCLUSION |
|------------------------|----------------|----------|------------|
| Altitude simulation    | N1~N4<br>C1~C4 | UN38.3   | PASS       |
| Thermal test           |                |          | PASS       |
| Vibration              |                |          | PASS       |
| Shock                  |                |          | PASS       |
| External short circuit |                |          | PASS       |
| Impact                 | N9~N13         |          | PASS       |
| Overcharge             | N5~N8 C5~C8    |          | PASS       |
| Forced discharge       | N14~N23 C9~C18 |          | PASS       |

The submitted battery and component cell were complied with the UN Manual of Tests and Criteria, Part III, sub-section 38.3.

Prepared by: *Pony Test*

Checked by: *chengpeng*

Approved by: *Lijun*

Approval Date: December 2, 2013



www.ponytest.com    ☎Hotline 400-819-5688

|                         |                           |                              |                      |
|-------------------------|---------------------------|------------------------------|----------------------|
| Add: 北京市朝阳区东三环49-3号智人大厦 | Add: 上海市徐汇区天平路690号35号楼4层  | Add: 深圳市福田区彩田路中兴C座408A室      | Add: 青岛市崂山区株洲路199号6层 |
| Tel: (010) 82618118     | Tel: (021) 64851999       | Tel: (0755) 26880088         | Tel: (0532) 89788800 |
| Add: 天津市南开区红旗路嘉里大厦109   | Add: 宁波市江北区新海路150号二单元404室 | Add: 广州市海珠区琶洲路189号海珠科技园3号楼7层 |                      |
| Tel: (022) 27340730     | Tel: (0574) 87736499      | Tel: (020) 89724315          |                      |